

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100121\
Data File : FF009059.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2021 13:53
Operator : DD\AJ
Sample : M3991-02 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MW-23-20210929-0-1-D

Integration File: autoint1.e
Quant Time: Oct 01 22:30:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	153013	1.303 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100121\
Data File : FF009059.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2021 13:53
Operator : DD\AJ
Sample : M3991-02 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MW-23-20210929-0-1-D

Integration File: autoint1.e
Quant Time: Oct 01 22:30:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

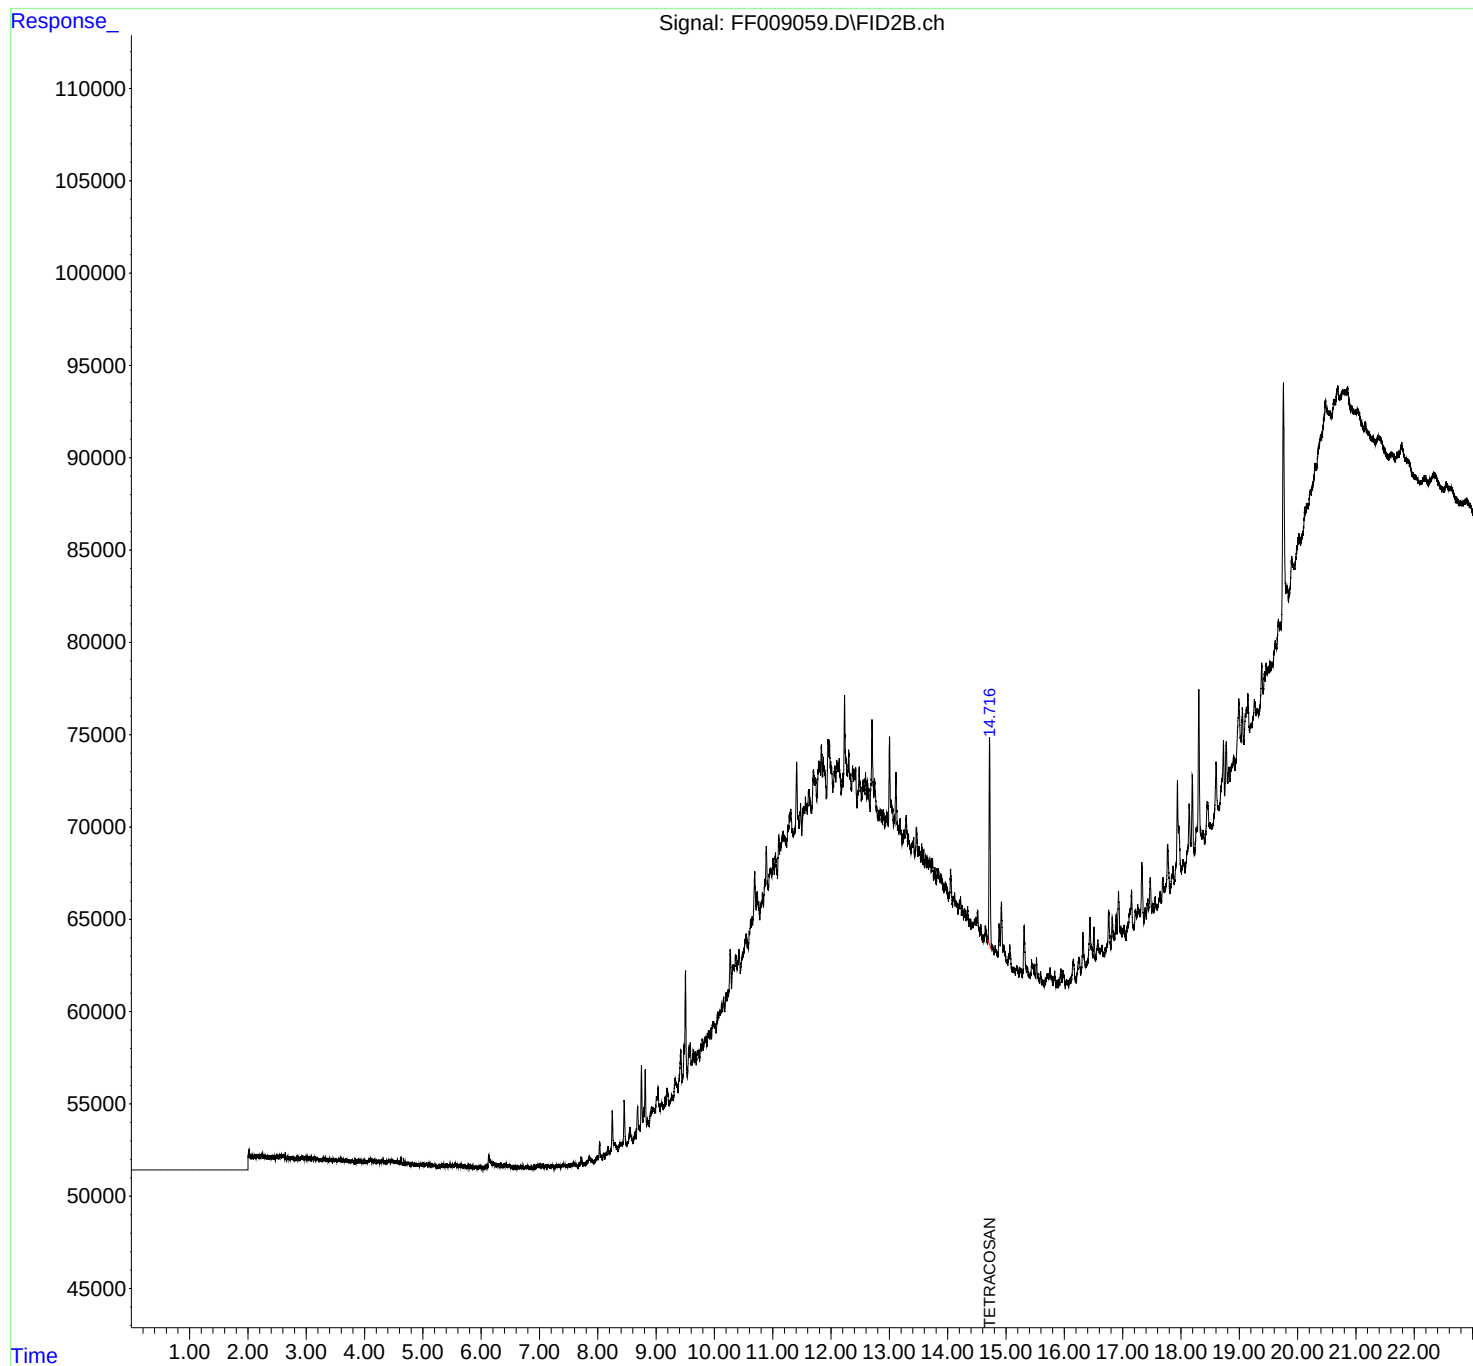

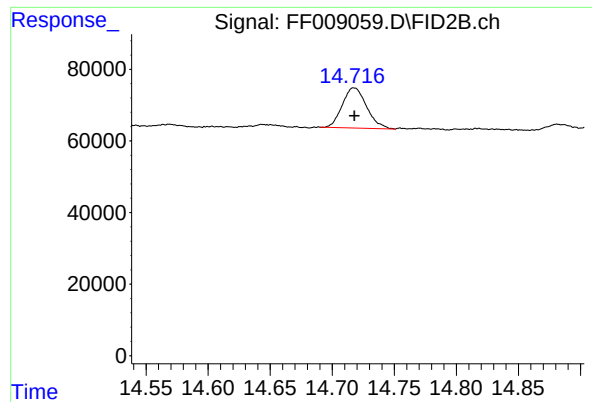

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.717 min
Delta R.T.: 0.000 min
Response: 153013
Conc: 1.30 ug/ml

Instrument :
FID_F
ClientSampleId :
MW-23-20210929-0-1-D