

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100218\
Data File : FF002308.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2018 13:02
Operator : AJ\SJ
Sample : J5155-03 50X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 05:15:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

1)	N-OCTANE	2.239	97062	0.614 ug/ml
2)	N-DECANE	4.413	431040	2.661 ug/ml
3)	N-DODECANE	6.408	372125	2.262 ug/ml
4)	N-TETRADECANE	8.159	165385	0.993 ug/ml
5)	N-HEXADECANE	9.805	222185	1.327 ug/ml
6)	N-OCTADECANE	11.250	204083	1.215 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100218\
Data File : FF002308.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2018 13:02
Operator : AJ\SJ
Sample : J5155-03 50X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 05:15:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

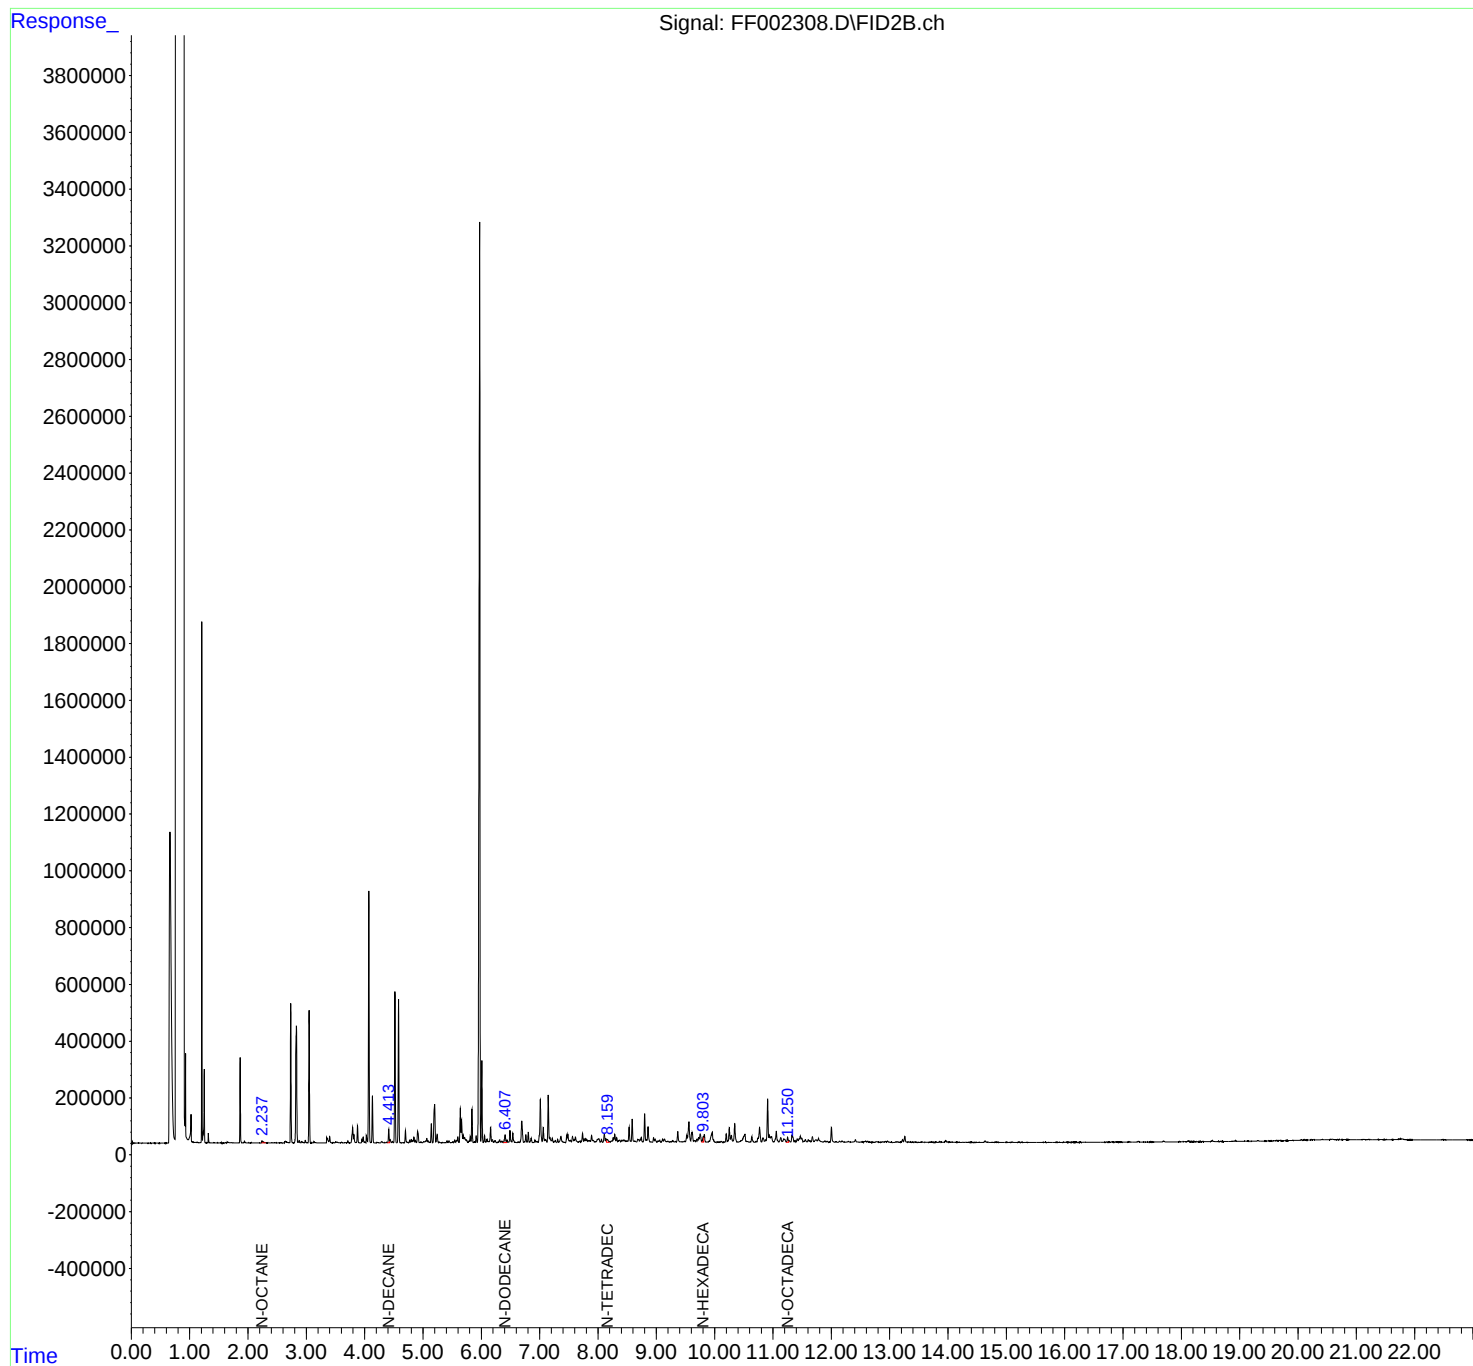


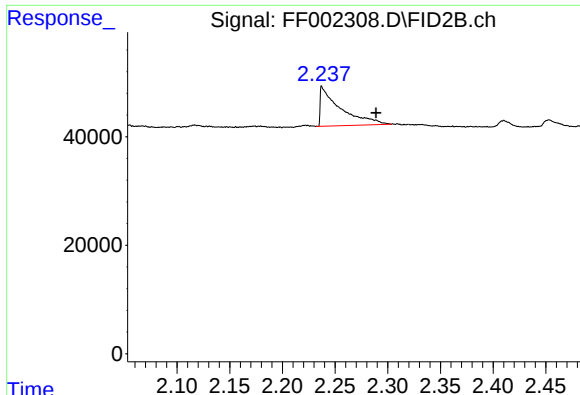

#1 N-OCTANE


R.T.: 2.239 min
Delta R.T.: -0.050 min
Response: 97062
Conc: 0.61 ug/ml

Instrument :
FID_F
ClientSampleId :

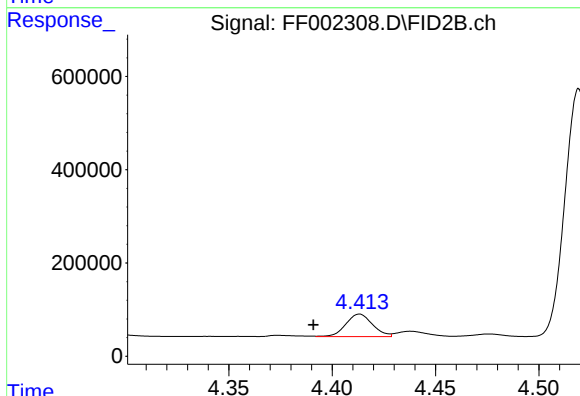


#2 N-DECANE

R.T.: 4.413 min
Delta R.T.: 0.022 min
Response: 431040
Conc: 2.66 ug/ml

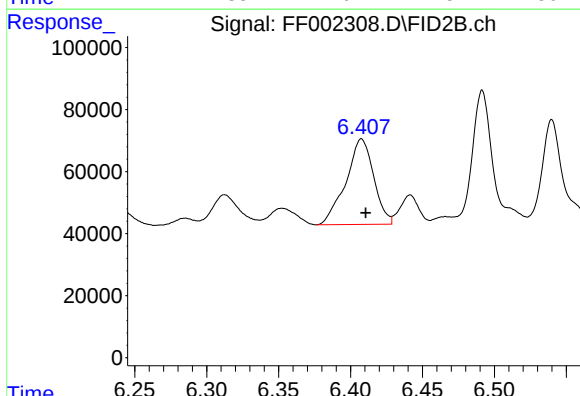


#3 N-DODECANE

R.T.: 6.408 min
Delta R.T.: -0.003 min
Response: 372125
Conc: 2.26 ug/ml

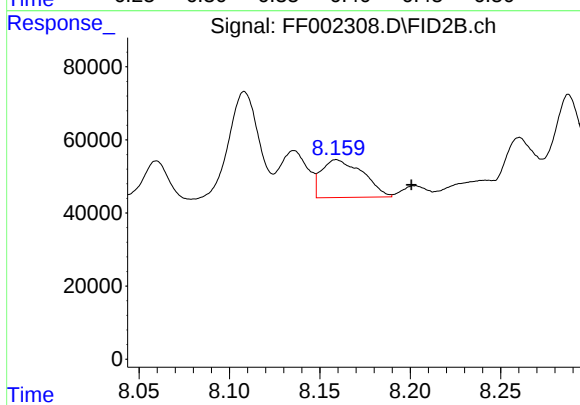

#4 N-TETRADECANE


R.T.: 8.159 min
Delta R.T.: -0.041 min
Response: 165385
Conc: 0.99 ug/ml

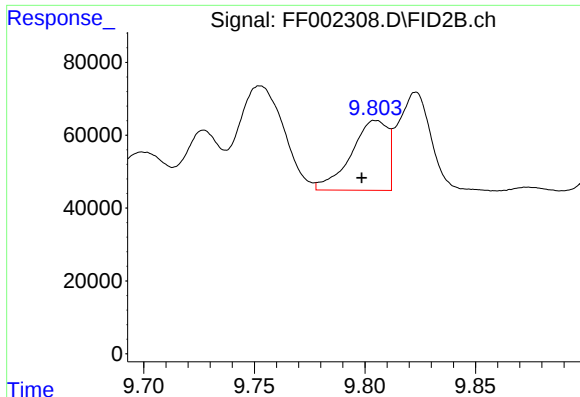

#5 N-HEXADECANE


R.T.: 9.805 min
Delta R.T.: 0.006 min
Response: 222185
Conc: 1.33 ug/ml

Instrument :
FID_F
ClientSampleId :

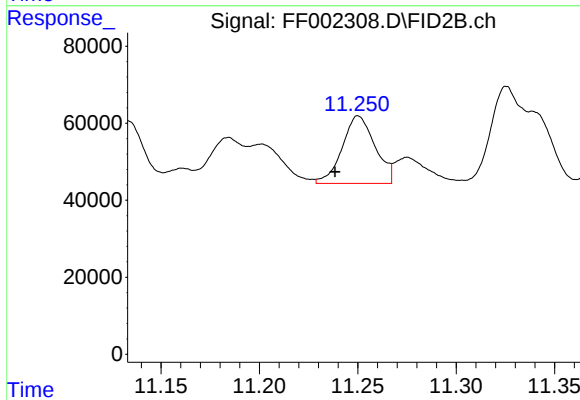

#6 N-OCTADECANE

R.T.: 11.250 min
Delta R.T.: 0.012 min
Response: 204083
Conc: 1.22 ug/ml

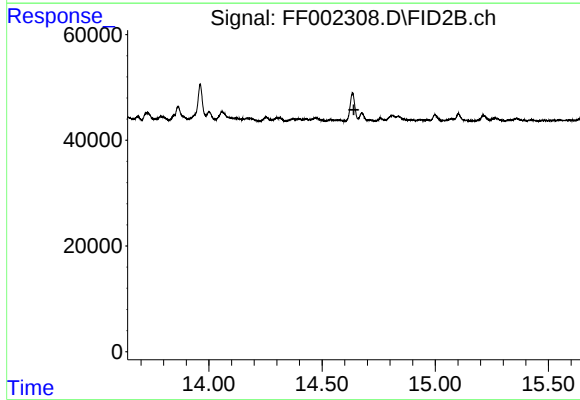

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.640 min
Response: 0
Conc: N.D.