

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100218\
Data File : FF002309.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2018 13:32
Operator : AJ\SJ
Sample : J5155-04 50X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 05:15:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.424	344232	2.125 ug/ml
4) N-TETRADECANE	8.208	101345	0.608 ug/ml
5) N-HEXADECANE	9.758	451959	2.699 ug/ml
6) N-OCTADECANE	11.254	279178	1.663 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100218\
Data File : FF002309.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2018 13:32
Operator : AJ\SJ
Sample : J5155-04 50X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 05:15:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

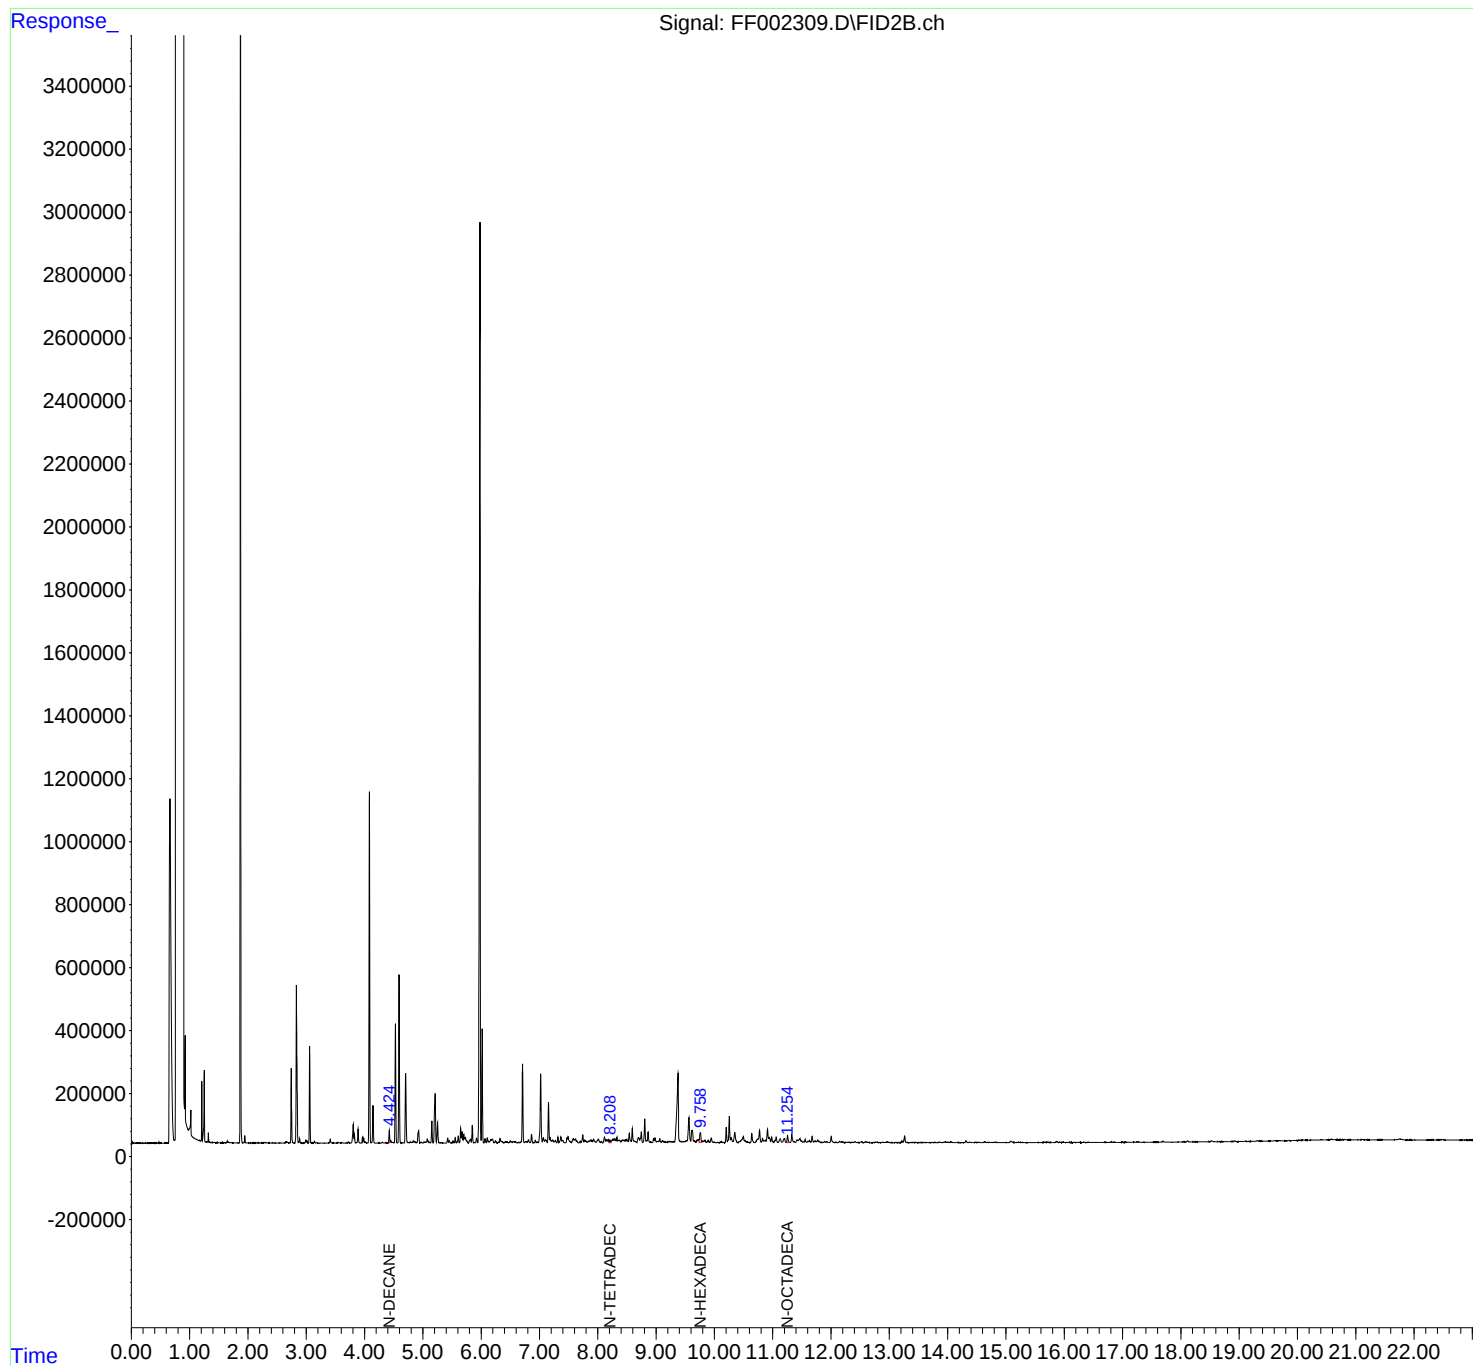


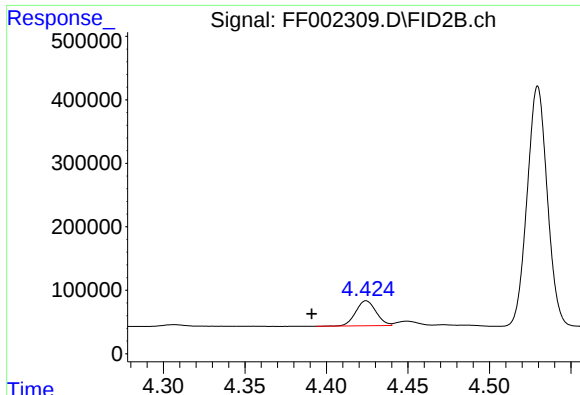

#2 N-DECANE


R.T.: 4.424 min
Delta R.T.: 0.034 min
Response: 344232
Conc: 2.13 ug/ml

Instrument :
FID_F
ClientSampleId :

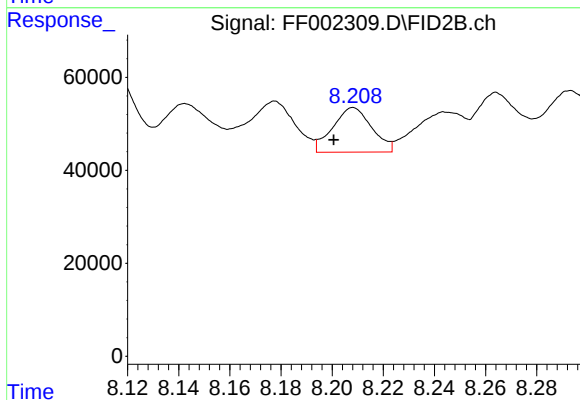


#4 N-TETRADECANE

R.T.: 8.208 min
Delta R.T.: 0.008 min
Response: 101345
Conc: 0.61 ug/ml

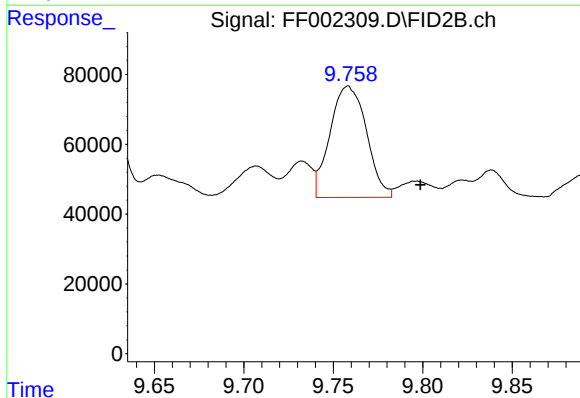


#5 N-HEXADECANE

R.T.: 9.758 min
Delta R.T.: -0.040 min
Response: 451959
Conc: 2.70 ug/ml

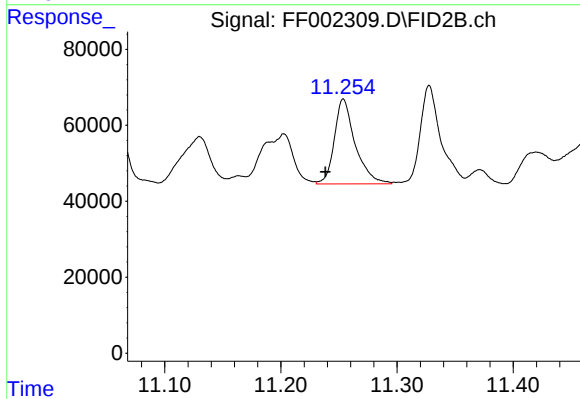

#6 N-OCTADECANE

R.T.: 11.254 min
Delta R.T.: 0.015 min
Response: 279178
Conc: 1.66 ug/ml

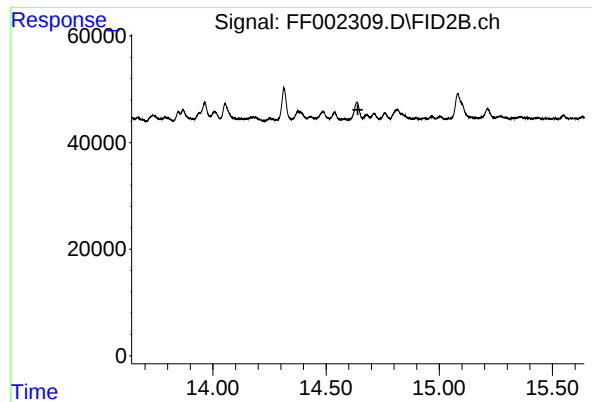

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.640 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :