

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100218\
Data File : FF002310.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2018 14:02
Operator : AJ\SJ
Sample : J5155-05 50X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 05:16:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.426	339558	2.096 ug/ml
4) N-TETRADECANE	8.230	219205	1.316 ug/ml
5) N-HEXADECANE	9.759	332720	1.987 ug/ml
6) N-OCTADECANE	11.254	183115	1.091 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100218\
Data File : FF002310.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2018 14:02
Operator : AJ\SJ
Sample : J5155-05 50X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 05:16:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

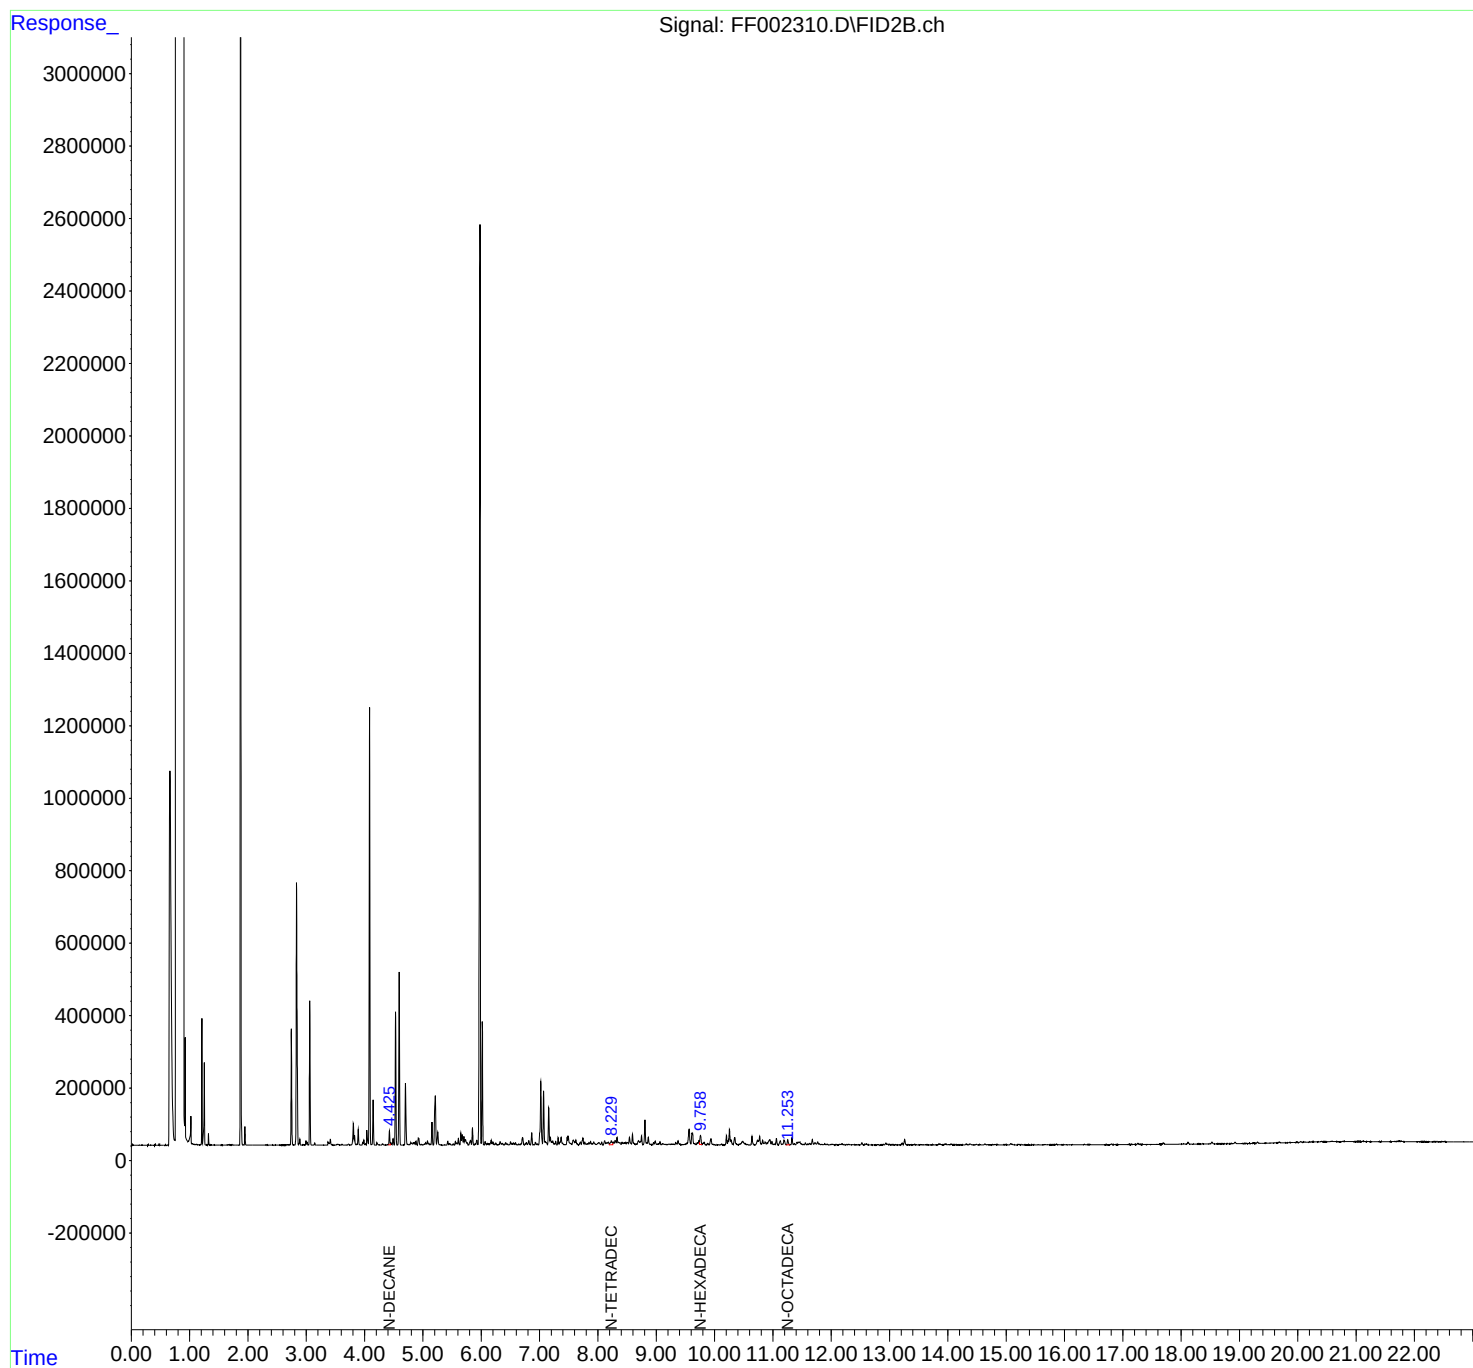


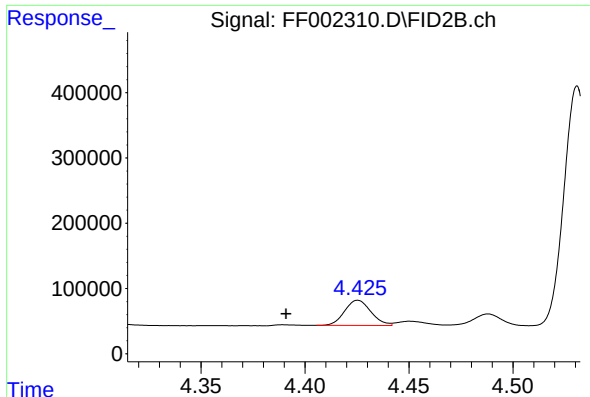

#2 N-DECANE


R.T.: 4.426 min
Delta R.T.: 0.035 min
Response: 339558
Conc: 2.10 ug/ml

Instrument :
FID_F
ClientSampleId :

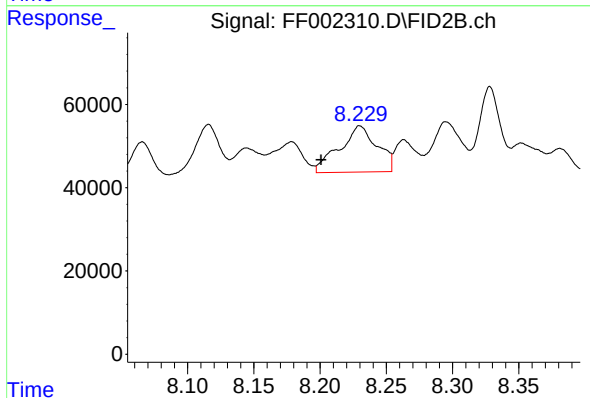


#4 N-TETRADECANE

R.T.: 8.230 min
Delta R.T.: 0.029 min
Response: 219205
Conc: 1.32 ug/ml

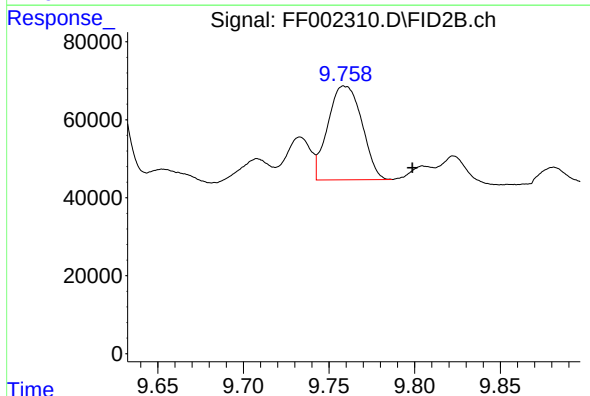


#5 N-HEXADECANE

R.T.: 9.759 min
Delta R.T.: -0.040 min
Response: 332720
Conc: 1.99 ug/ml

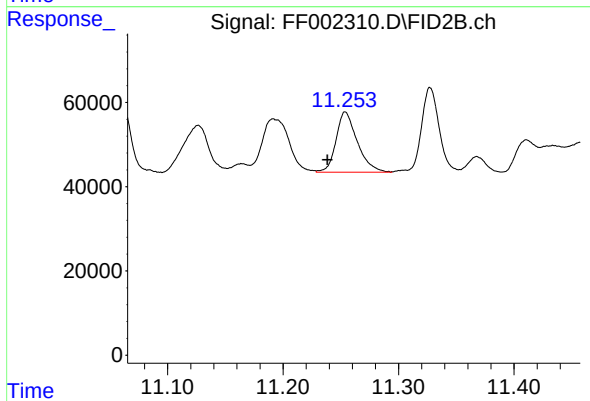

#6 N-OCTADECANE

R.T.: 11.254 min
Delta R.T.: 0.016 min
Response: 183115
Conc: 1.09 ug/ml

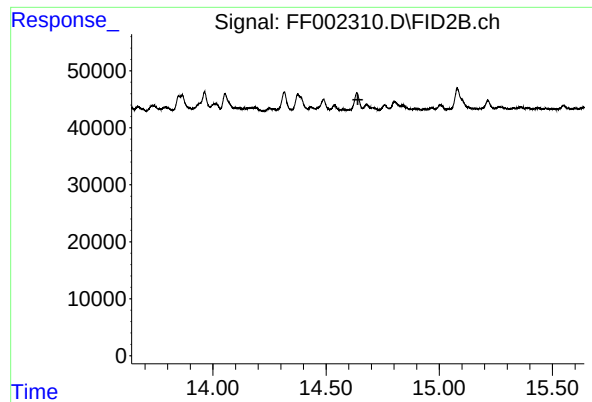

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.640 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :