

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100218\
 Data File : FF002312.D
 Signal(s) : FID2B.ch
 Acq On : 02 Oct 2018 15:04
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 03 05:16:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.643	6972611	48.888 ug/ml
Target Compounds			
2) N-DECANE	4.387	8228355	50.796 ug/ml
3) N-DODECANE	6.406	8336592	50.677 ug/ml
4) N-TETRADECANE	8.198	8391557	50.377 ug/ml
5) N-HEXADECANE	9.797	8394021	50.122 ug/ml
6) N-OCTADECANE	11.238	8361998	49.801 ug/ml
7) N-EICOSANE	12.546	8186413	49.430 ug/ml
8) N-DOCOSANE	13.744	7995033	48.998 ug/ml
10) N-TETRACOSANE	14.847	7759128	48.525 ug/ml
11) N-HEXACOSANE	15.866	7541718	48.151 ug/ml
12) N-OCTACOSANE	16.816	7316515	47.830 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100218\
Data File : FF002312.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2018 15:04
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 05:16:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

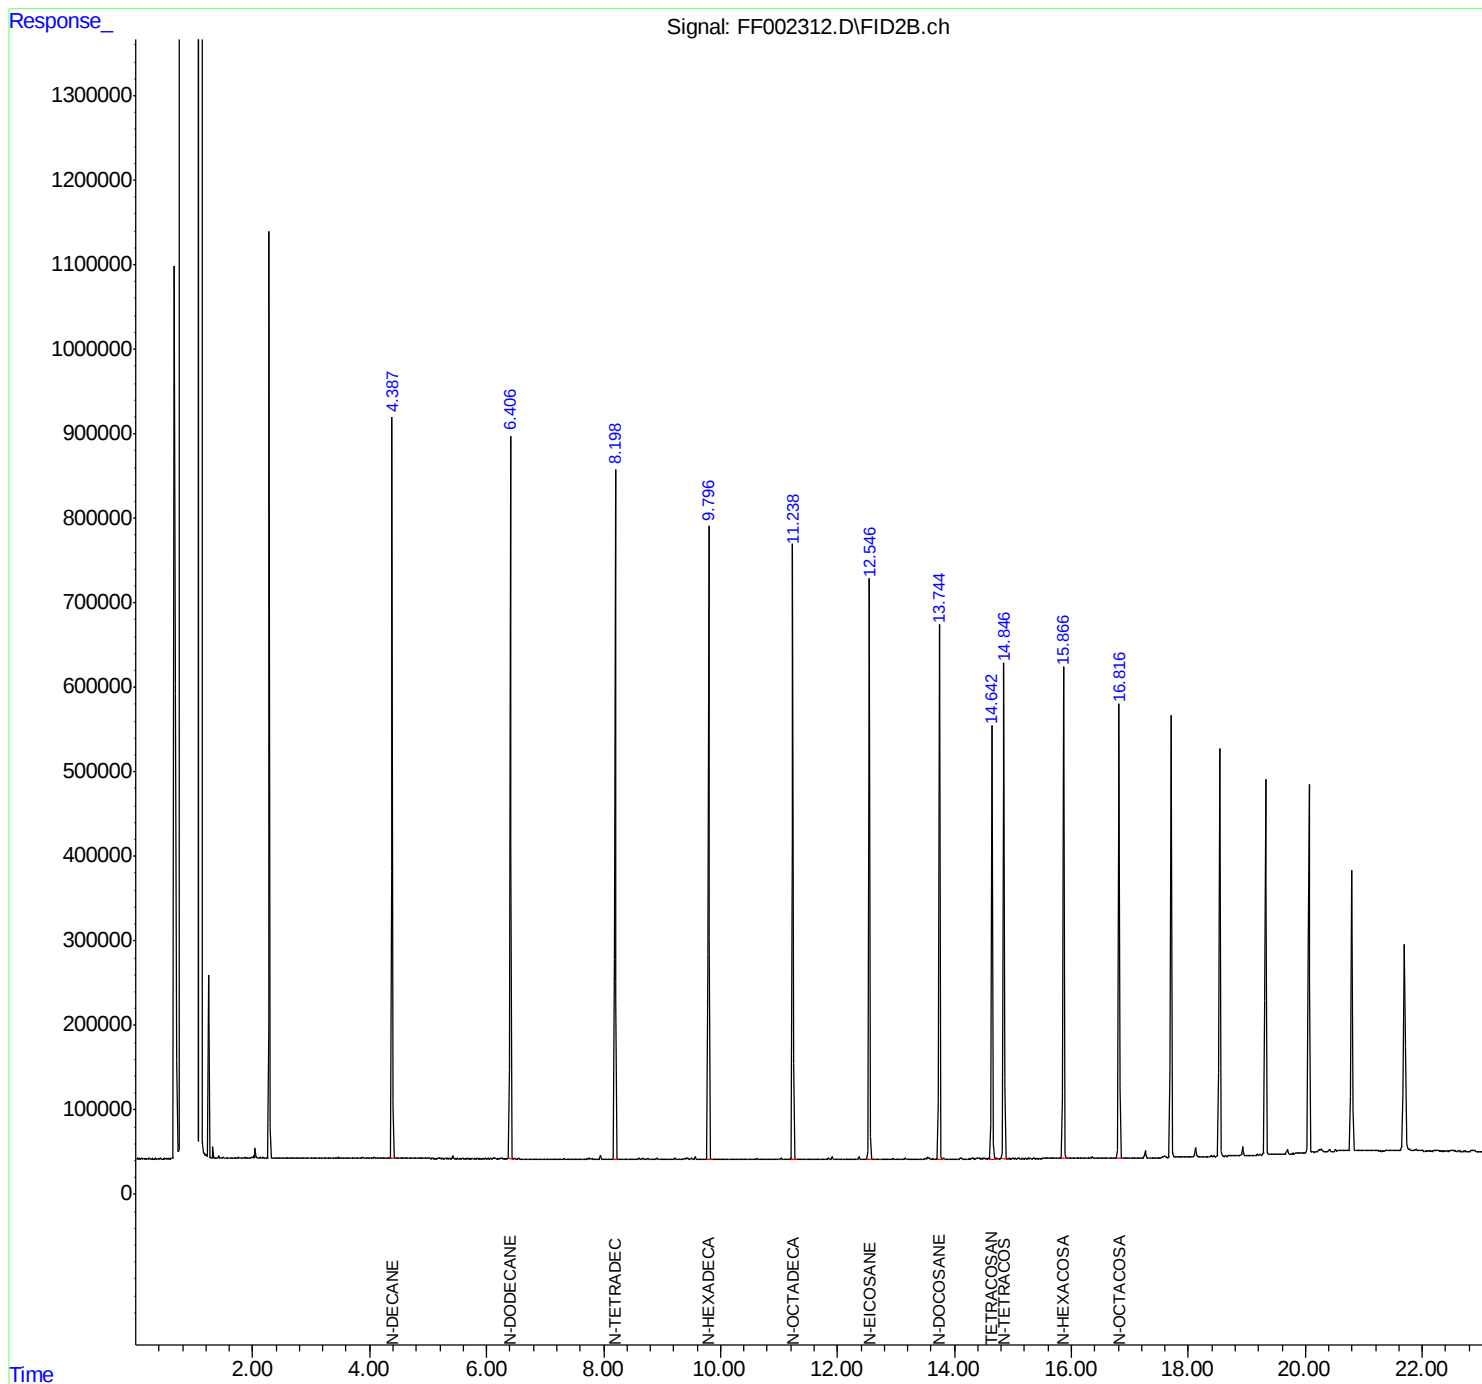


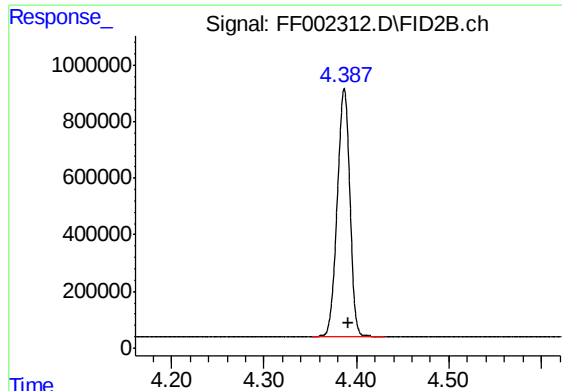

#2 N-DECANE


R.T.: 4.387 min
Delta R.T.: -0.004 min
Response: 8228355
Conc: 50.80 ug/ml

Instrument :
FID_F
ClientSampleId :

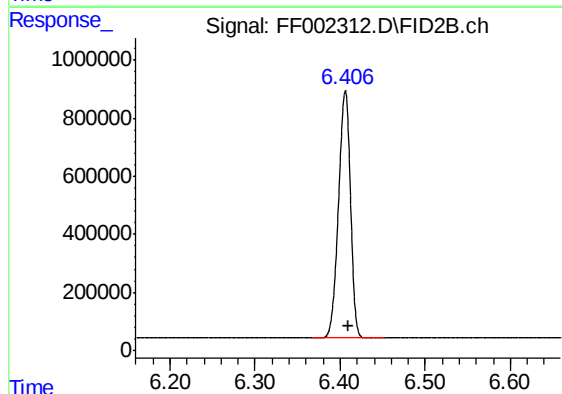


#3 N-DODECANE

R.T.: 6.406 min
Delta R.T.: -0.004 min
Response: 8336592
Conc: 50.68 ug/ml

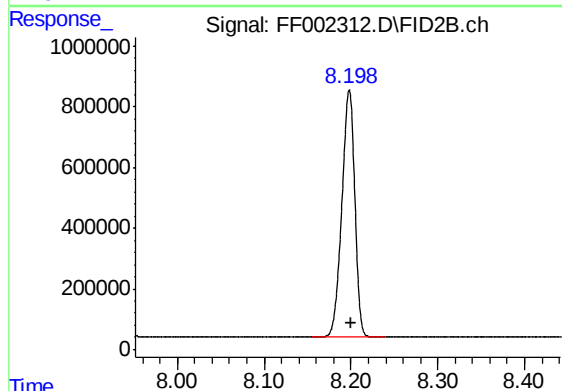


#4 N-TETRADECANE

R.T.: 8.198 min
Delta R.T.: -0.002 min
Response: 8391557
Conc: 50.38 ug/ml

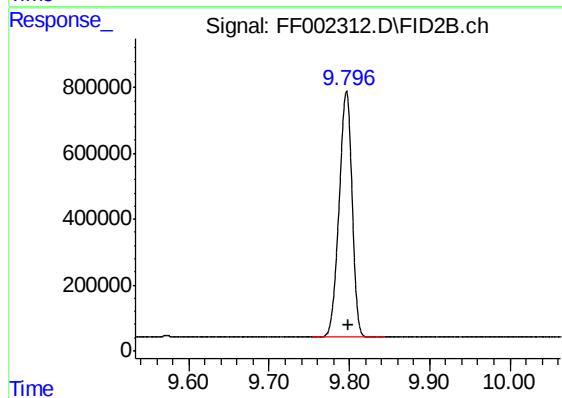

#5 N-HEXADECANE


R.T.: 9.797 min
Delta R.T.: -0.002 min
Response: 8394021
Conc: 50.12 ug/ml

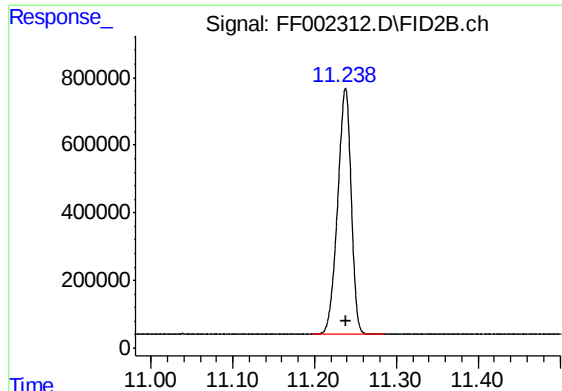

#6 N-OCTADECANE


R.T.: 11.238 min
Delta R.T.: 0.000 min
Response: 8361998
Conc: 49.80 ug/ml

Instrument :
FID_F
ClientSampleId :

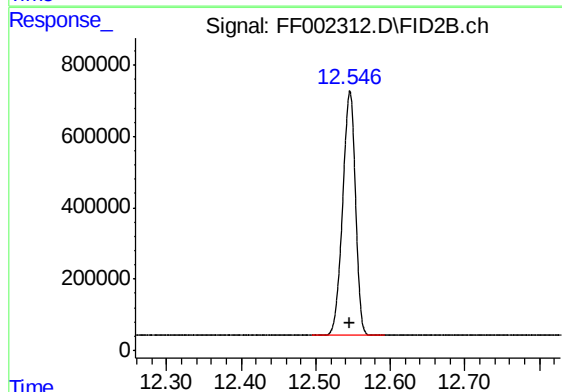


#7 N-EICOSANE

R.T.: 12.546 min
Delta R.T.: 0.000 min
Response: 8186413
Conc: 49.43 ug/ml

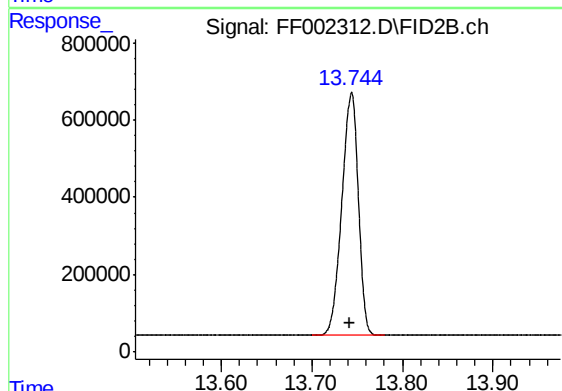


#8 N-DOCOSANE

R.T.: 13.744 min
Delta R.T.: 0.001 min
Response: 7995033
Conc: 49.00 ug/ml

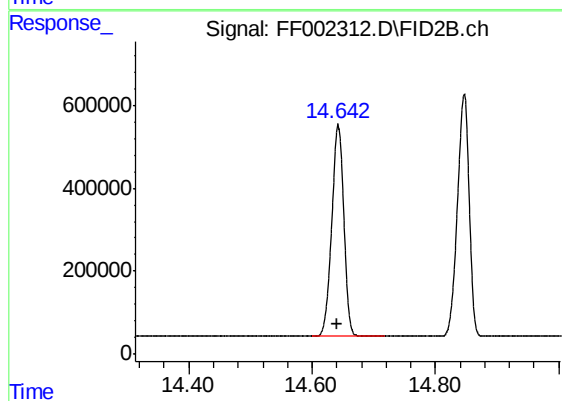

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.643 min
Delta R.T.: 0.002 min
Response: 6972611
Conc: 48.89 ug/ml

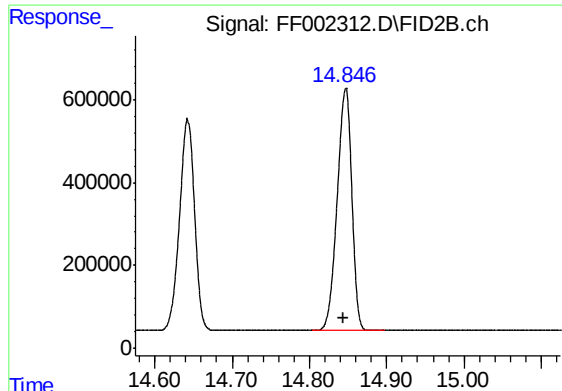

#10 N-TETRACOSANE


R.T.: 14.847 min
Delta R.T.: 0.003 min
Response: 7759128
Conc: 48.52 ug/ml

Instrument :
FID_F
ClientSampleId :

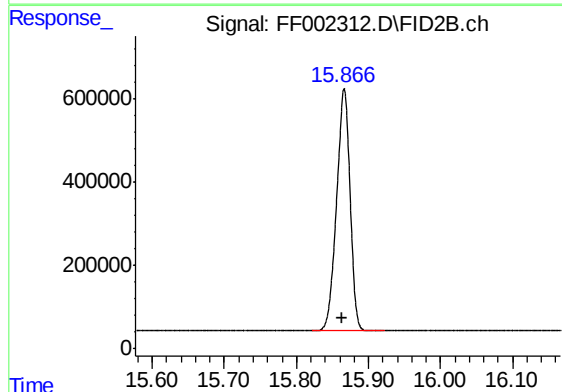

#11 N-HEXACOSANE

R.T.: 15.866 min
Delta R.T.: 0.003 min
Response: 7541718
Conc: 48.15 ug/ml

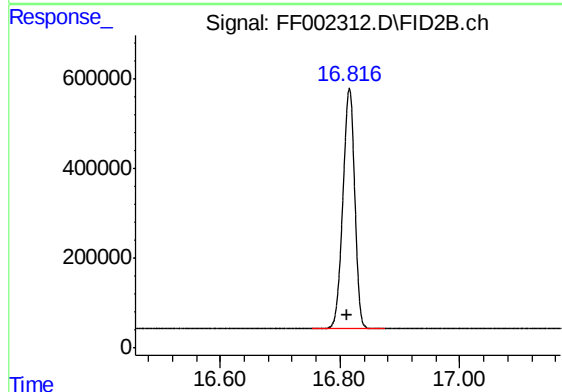

#12 N-OCTACOSANE

R.T.: 16.816 min
Delta R.T.: 0.003 min
Response: 7316515
Conc: 47.83 ug/ml