

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100219\
Data File : FF005712.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2019 14:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 03 04:28:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
Quant Title :
QLast Update : Thu Oct 03 04:07:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.680	2882928	22.173 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.604	826696	6.169 ug/ml
16) N-HEXATRIACONTANE	20.158f	2784840	25.786 ug/ml
18) N-TETRACONTANE	21.809f	3417431	30.474 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100219\
Data File : FF005712.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2019 14:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 03 04:28:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
Quant Title :
QLast Update : Thu Oct 03 04:07:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

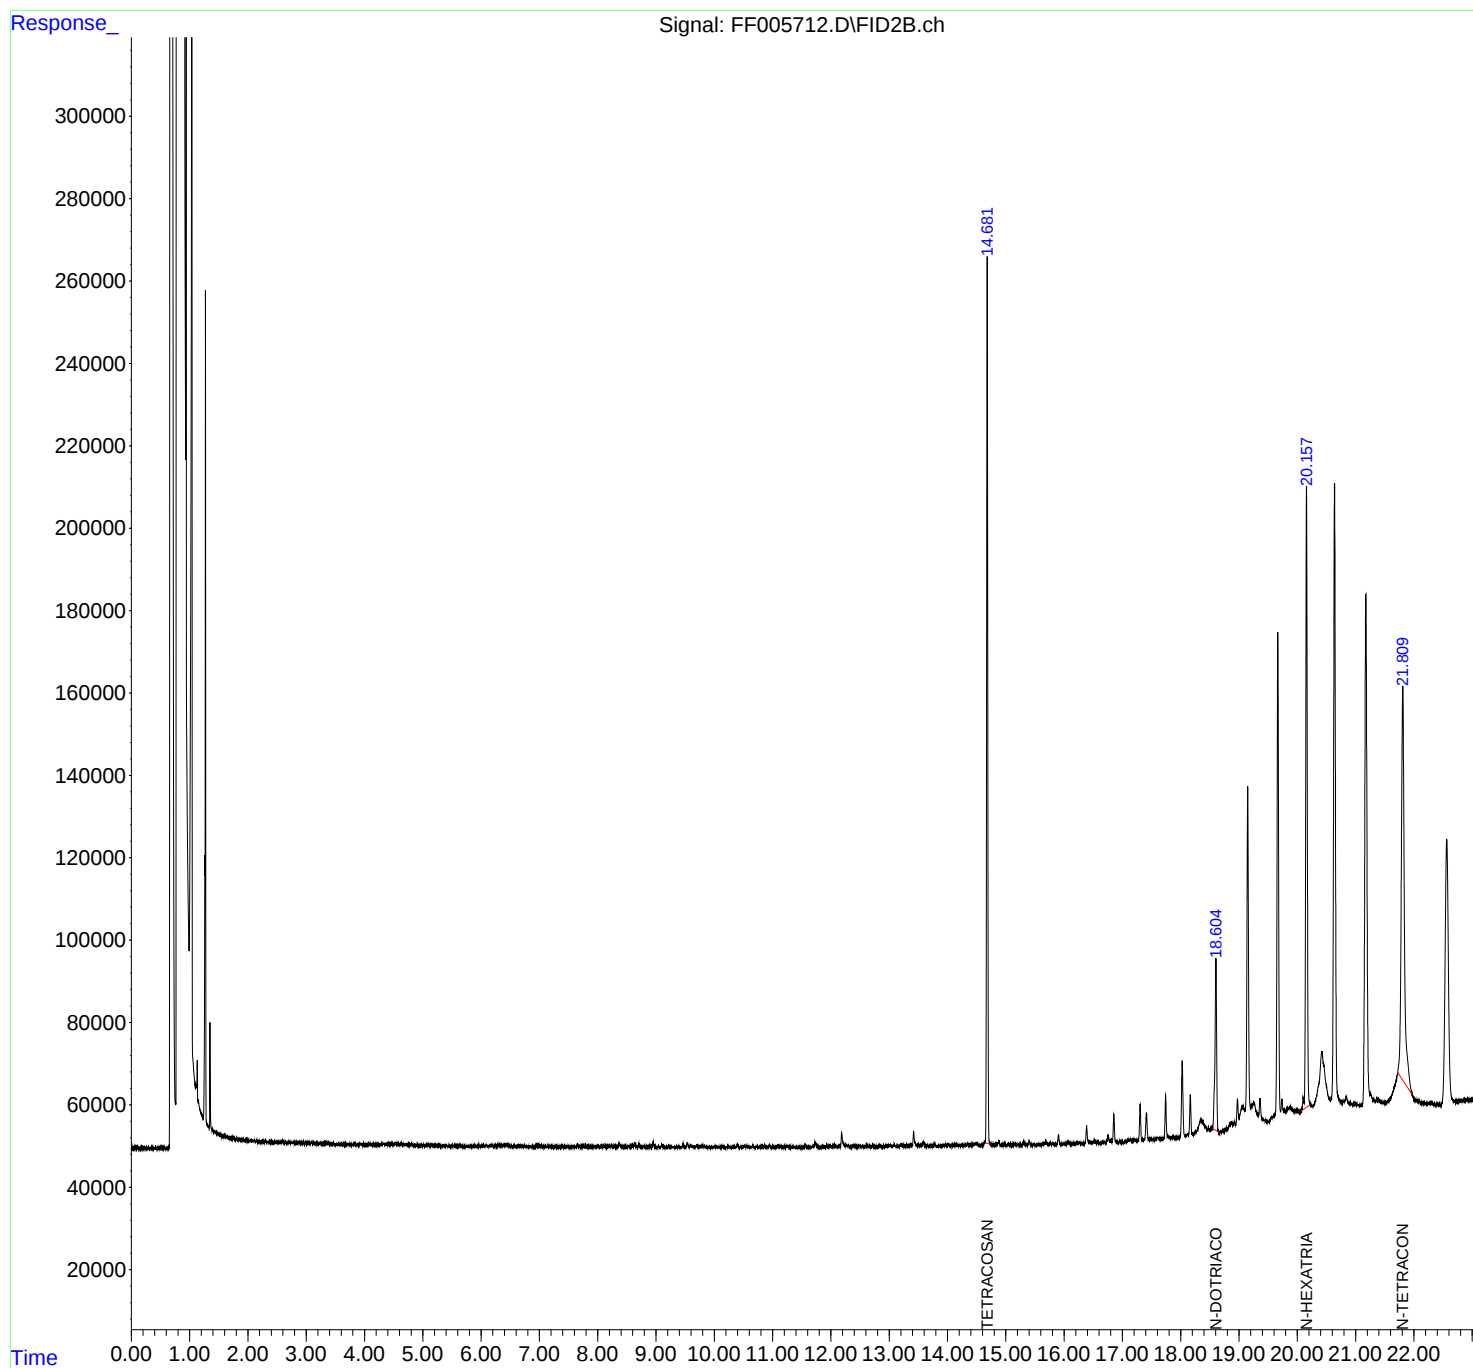


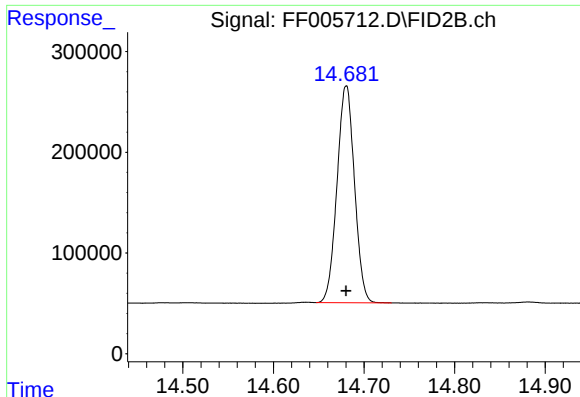

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.680 min
Delta R.T.: 0.000 min
Response: 2882928
Conc: 22.17 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

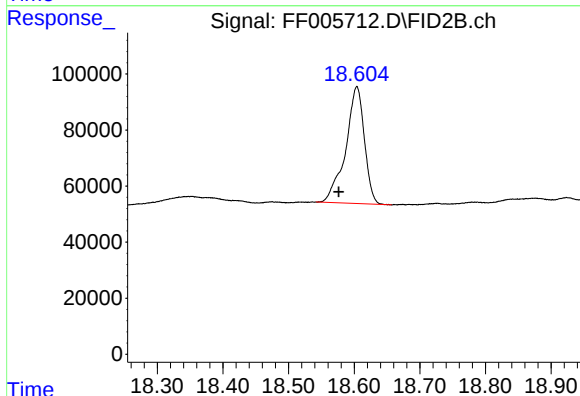


#14 N-DOTRIACONTANE

R.T.: 18.604 min
Delta R.T.: 0.028 min
Response: 826696
Conc: 6.17 ug/ml

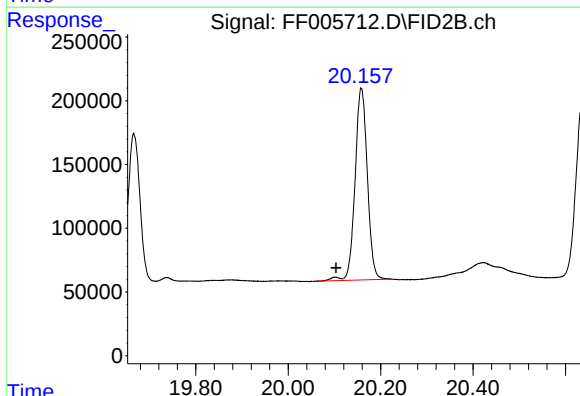

#16 N-HEXATRIACONTANE

R.T.: 20.158 min
Delta R.T.: 0.055 min
Response: 2784840
Conc: 25.79 ug/ml

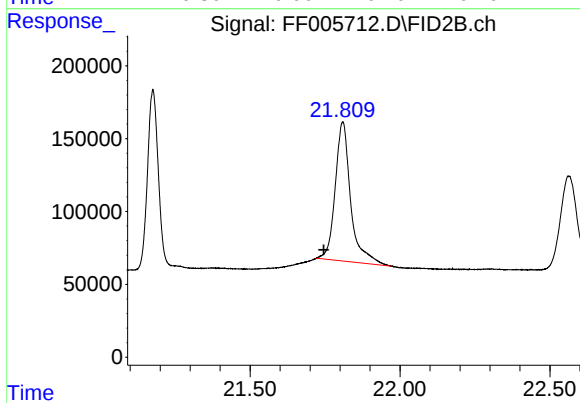

#18 N-TETRACONTANE

R.T.: 21.809 min
Delta R.T.: 0.063 min
Response: 3417431
Conc: 30.47 ug/ml