

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100220\
Data File : FF007684.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2020 18:59
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 05 15:35:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:32:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.639	117931	0.996 ug/ml
16)	N-HEXATRIACONTANE	20.201	285016	2.939 ug/ml
18)	N-TETRACONTANE	21.898	456923	5.047 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100220\
Data File : FF007684.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2020 18:59
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 05 15:35:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:32:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

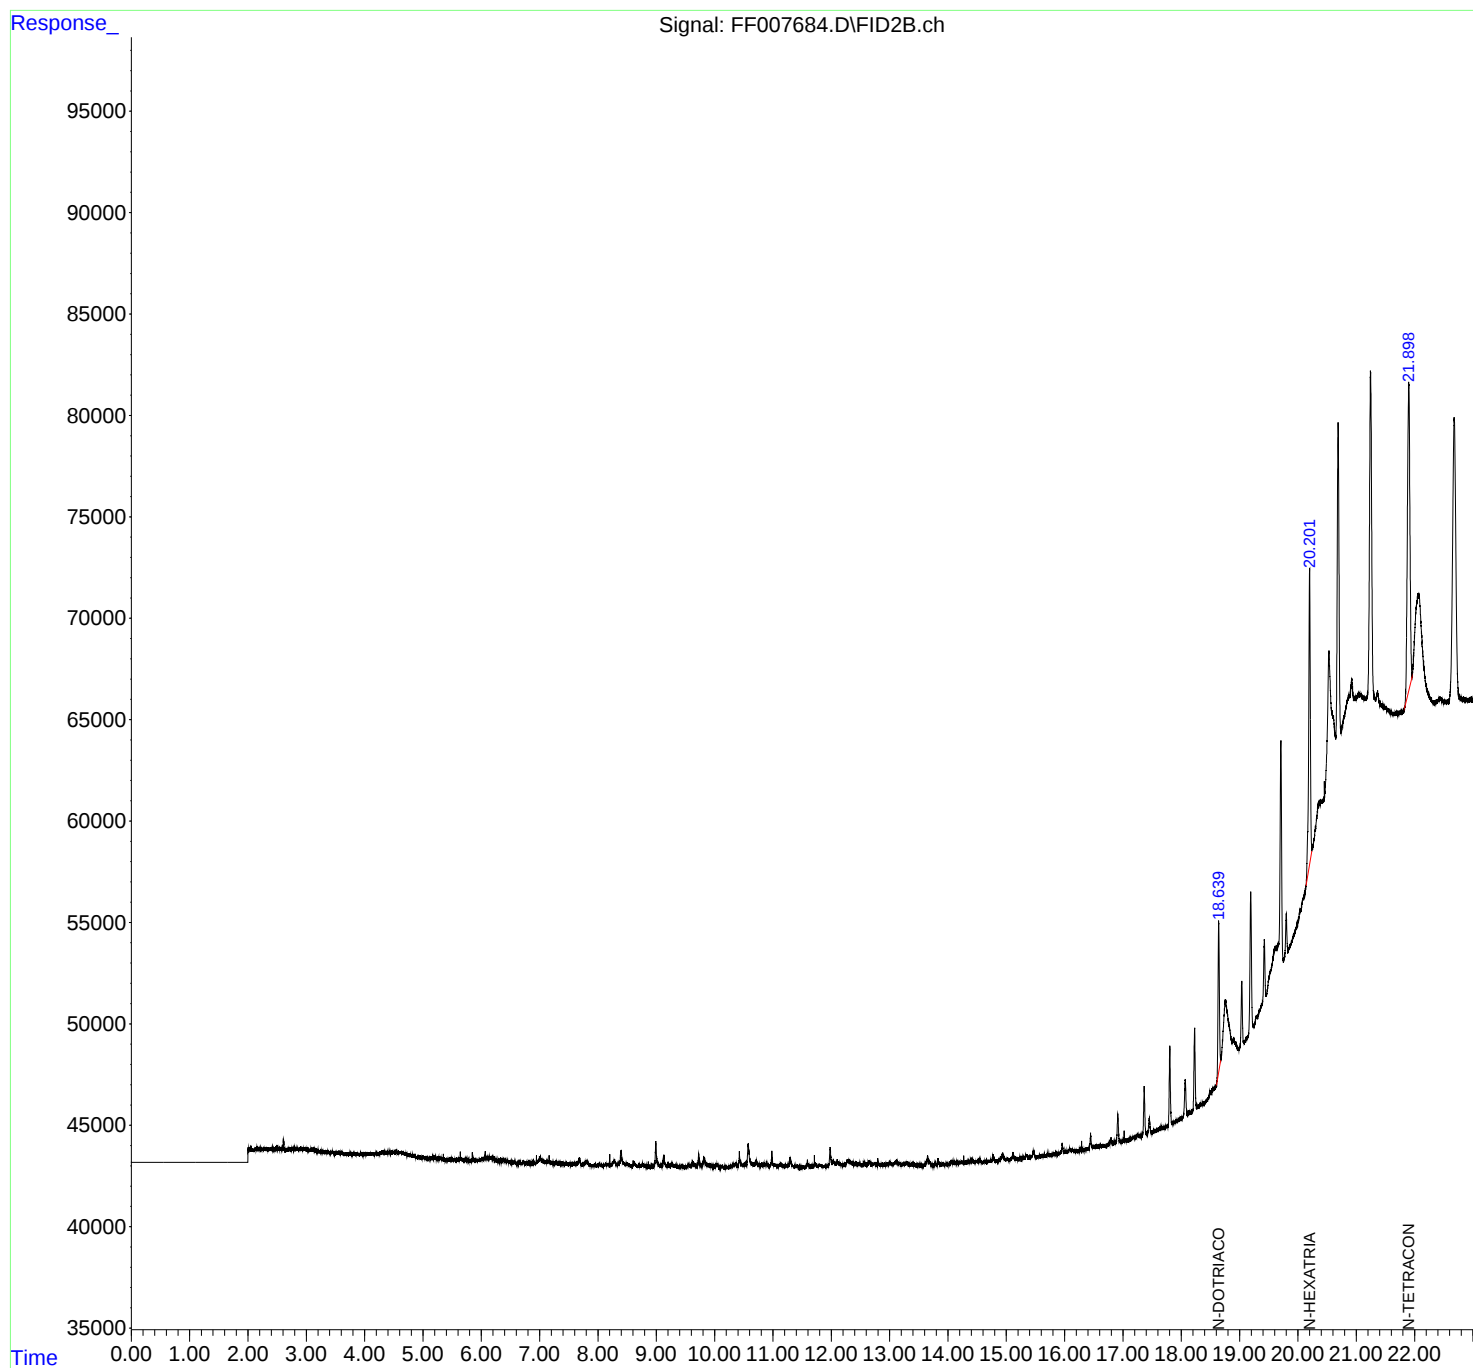


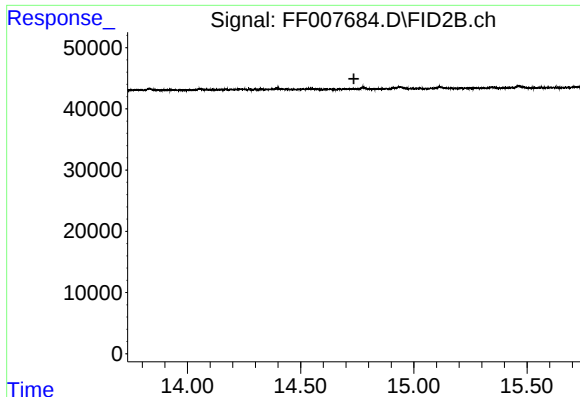

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.735 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

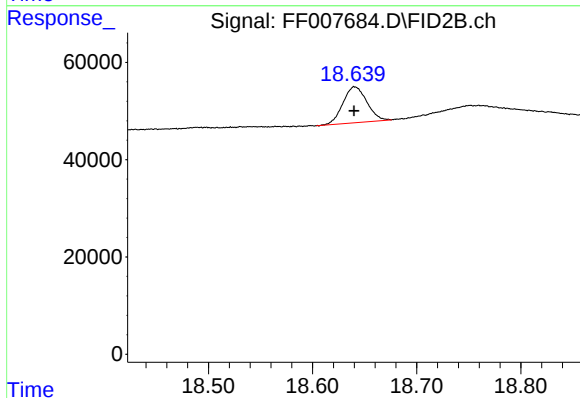


#14 N-DOTRIACONTANE

R.T.: 18.639 min
Delta R.T.: 0.000 min
Response: 117931
Conc: 1.00 ug/ml

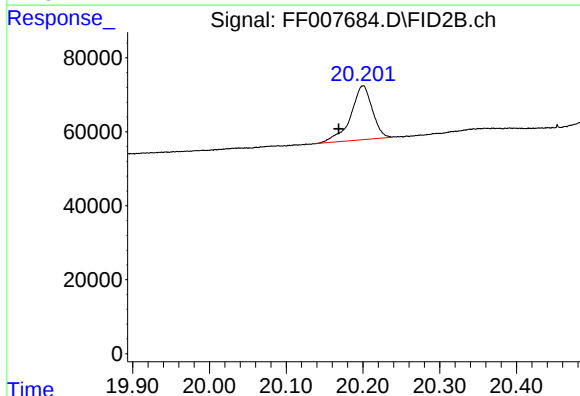

#16 N-HEXATRIACONTANE

R.T.: 20.201 min
Delta R.T.: 0.033 min
Response: 285016
Conc: 2.94 ug/ml

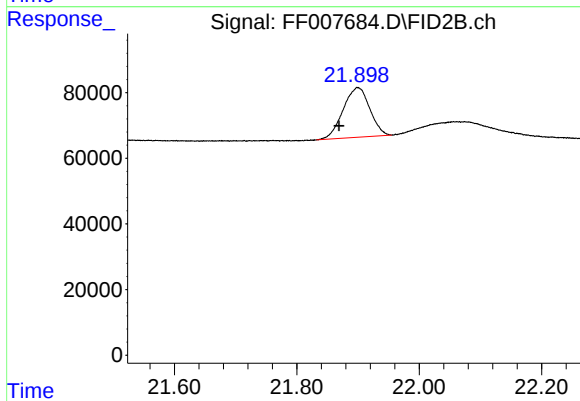

#18 N-TETRACONTANE

R.T.: 21.898 min
Delta R.T.: 0.029 min
Response: 456923
Conc: 5.05 ug/ml