

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100224\
Data File : FF014598.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2024 16:03
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 04:10:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100224.M
Quant Title :
QLast Update : Thu Oct 03 04:09:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.802	63578	0.469 ug/ml
16) N-HEXATRIACONTANE	20.350f	190155	1.595 ug/ml
18) N-TETRACONTANE	21.933f	173676	1.965 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100224\
Data File : FF014598.D
Signal(s) : FID2B.ch
Acq On : 02 Oct 2024 16:03
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 04:10:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100224.M
Quant Title :
QLast Update : Thu Oct 03 04:09:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

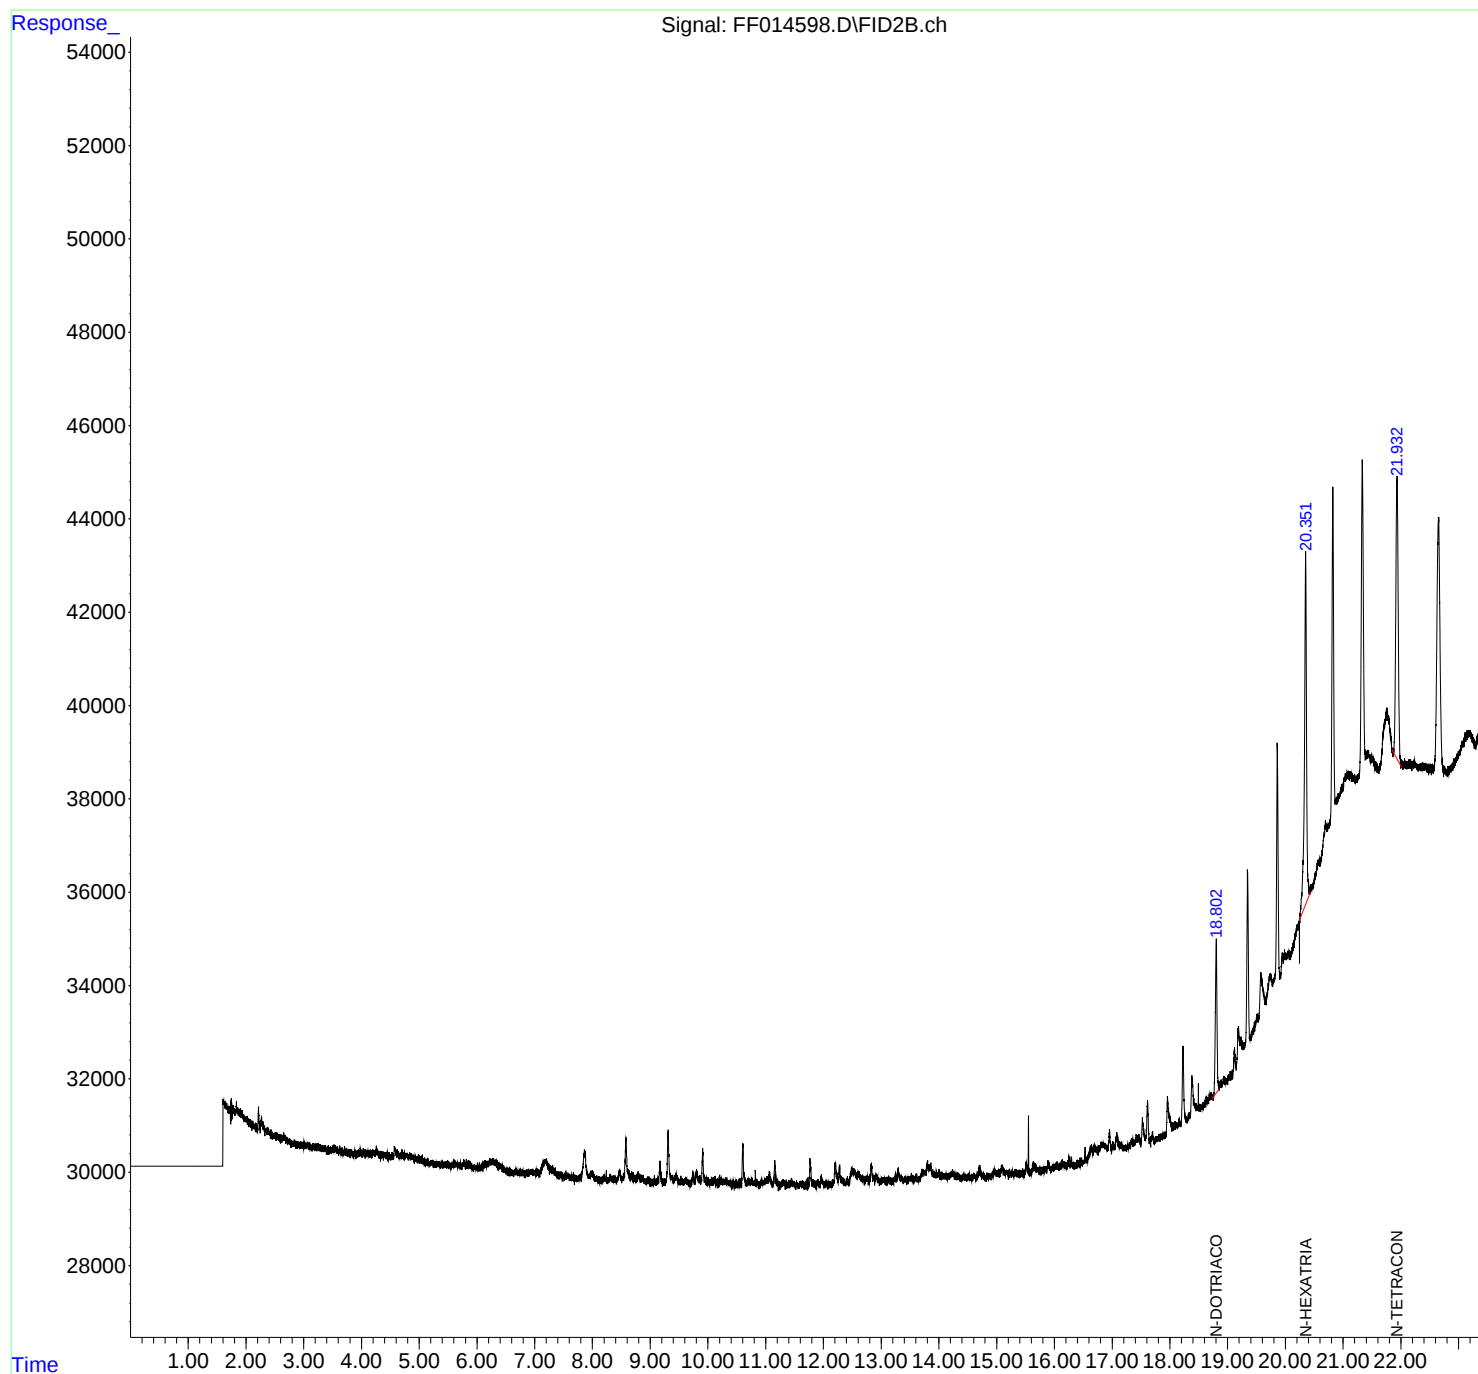


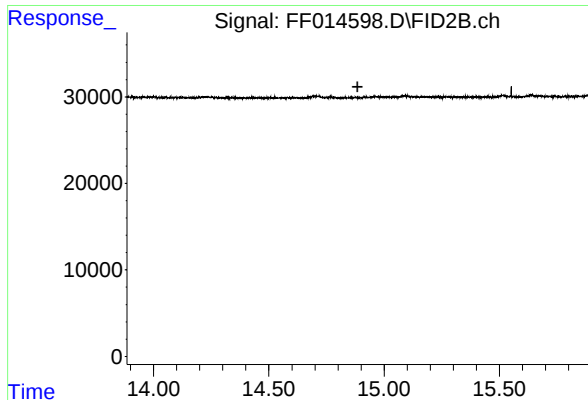

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.885 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

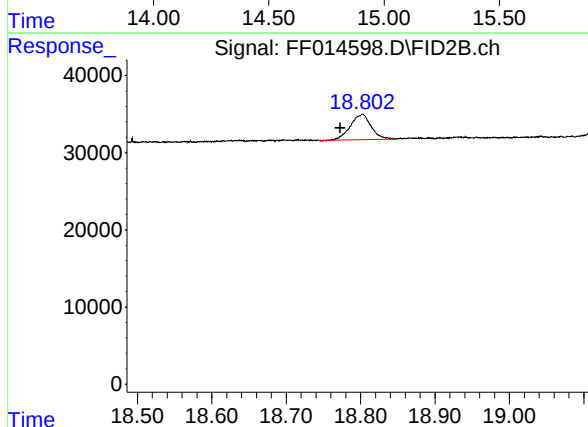


#14 N-DOTRIACONTANE

R.T.: 18.802 min
Delta R.T.: 0.029 min
Response: 63578
Conc: 0.47 ug/ml

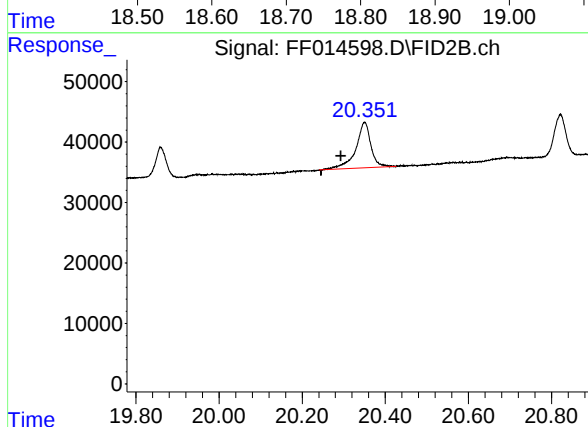

#16 N-HEXATRIACONTANE

R.T.: 20.350 min
Delta R.T.: 0.057 min
Response: 190155
Conc: 1.60 ug/ml

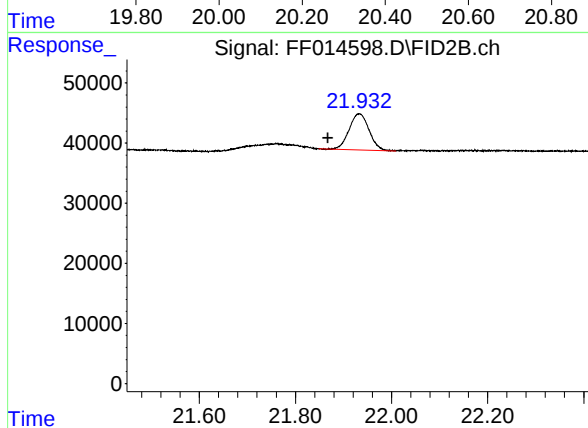

#18 N-TETRACONTANE

R.T.: 21.933 min
Delta R.T.: 0.065 min
Response: 173676
Conc: 1.96 ug/ml