

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100318\
 Data File : FF002324.D
 Signal(s) : FID2B.ch
 Acq On : 03 Oct 2018 18:39
 Operator : AJ\SJ
 Sample : J5200-03MS 5X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 04 04:56:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.646	569641	3.994 ug/ml
Target Compounds			
2) N-DECANE	4.388	455054	2.809 ug/ml
3) N-DODECANE	6.408	506310	3.078 ug/ml
4) N-TETRADECANE	8.199	574754	3.450 ug/ml
5) N-HEXADECANE	9.798	585829	3.498 ug/mlm
6) N-OCTADECANE	11.239	491248	2.926 ug/mlm
7) N-EICOSANE	12.549	482169	2.911 ug/mlm
8) N-DOCOSANE	13.748	703848	4.314 ug/ml
10) N-TETRACOSANE	14.850	514046	3.215 ug/ml
11) N-HEXACOSANE	15.871	519309	3.316 ug/mlm
12) N-OCTACOSANE	16.820	572759	3.744 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100318\
Data File : FF002324.D
Signal(s) : FID2B.ch
Acq On : 03 Oct 2018 18:39
Operator : AJ\SJ
Sample : J5200-03MS 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 04 04:56:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

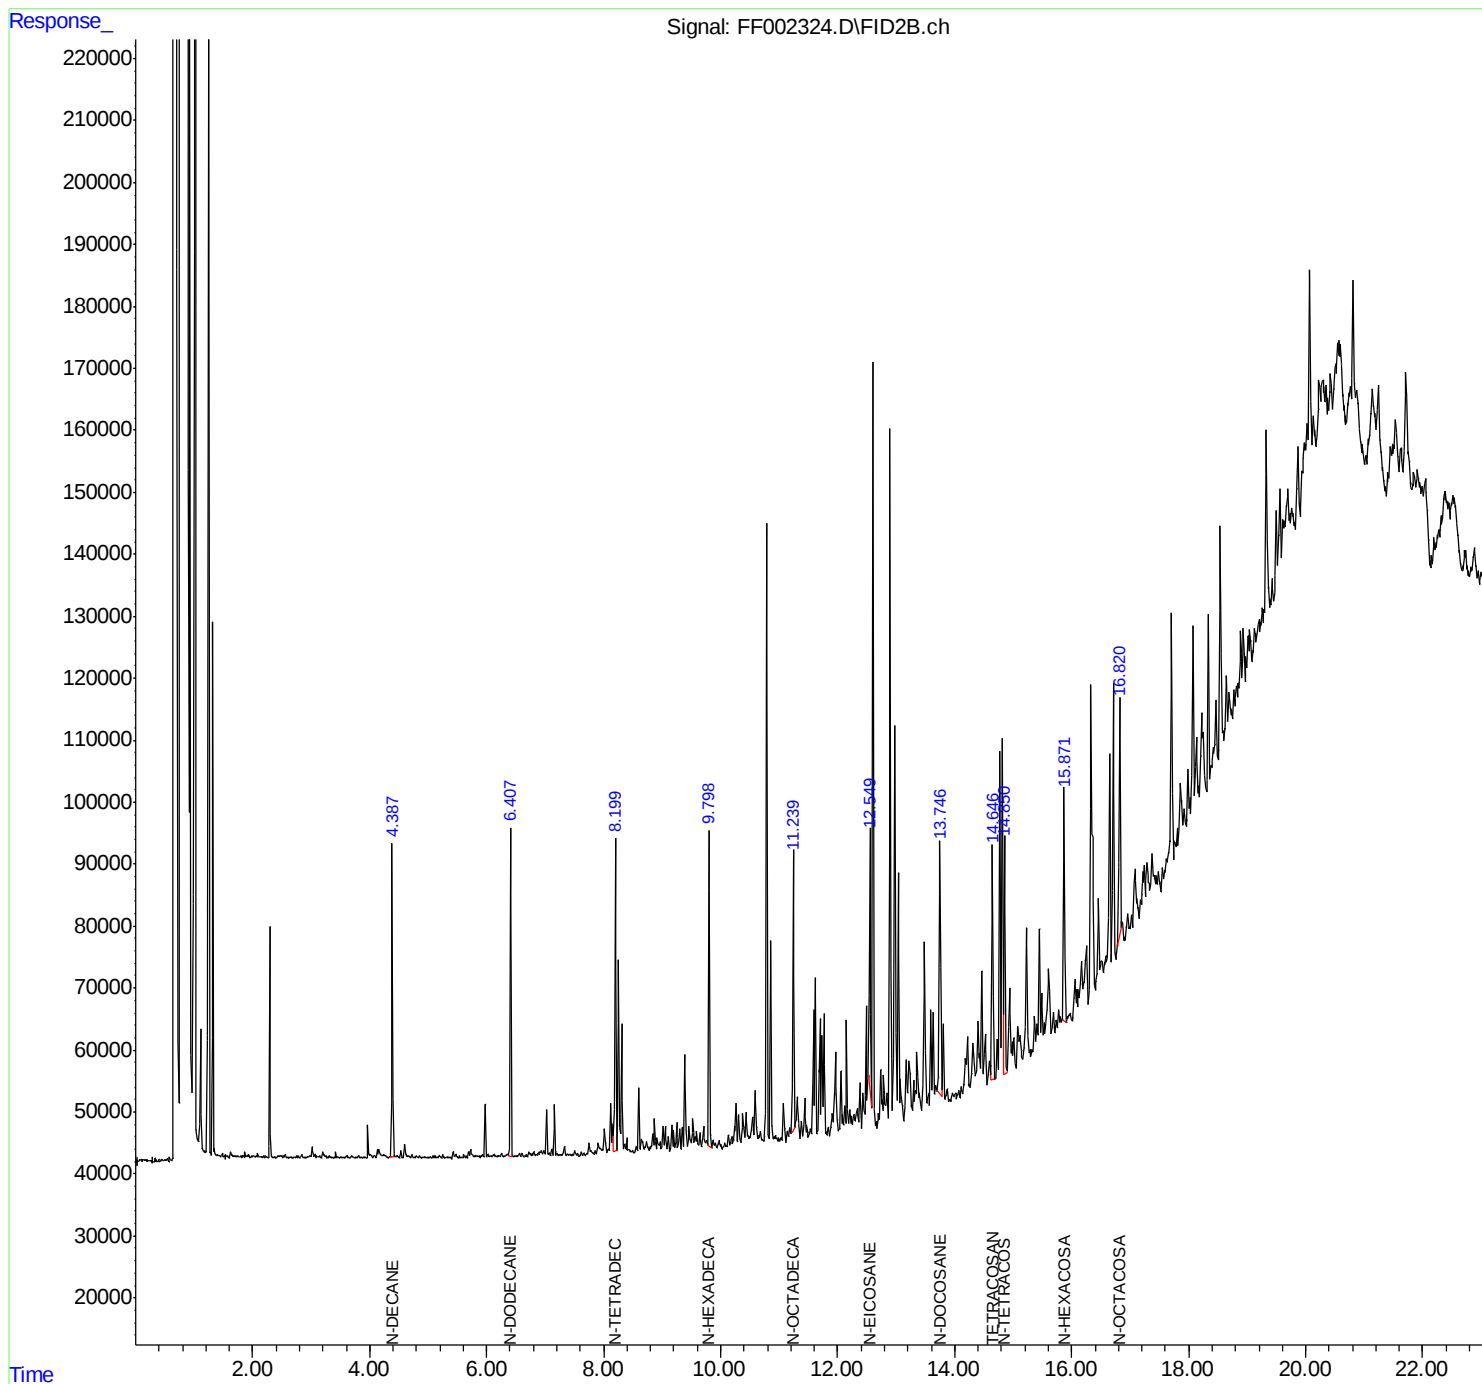

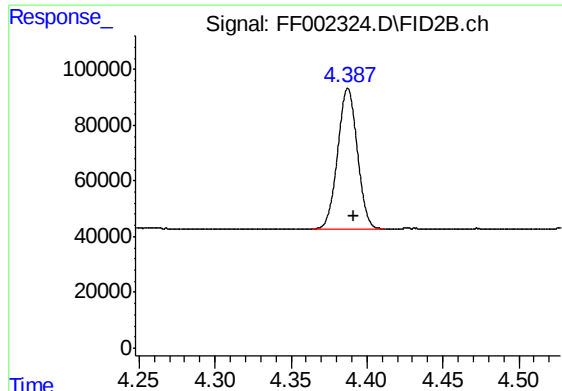


#2 N-DECANE

R.T.: 4.388 min
Delta R.T.: -0.003 min
Response: 455054
Conc: 2.81 ug/ml

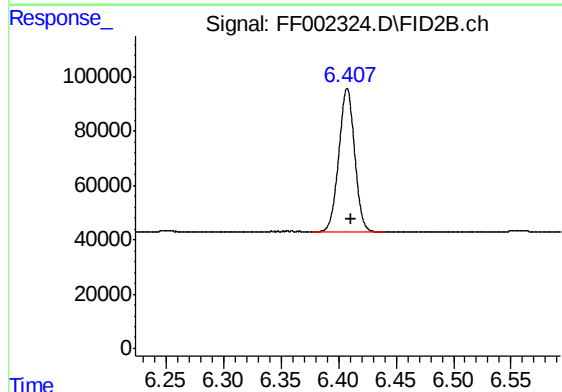


#3 N-DODECANE

R.T.: 6.408 min
Delta R.T.: -0.003 min
Response: 506310
Conc: 3.08 ug/ml

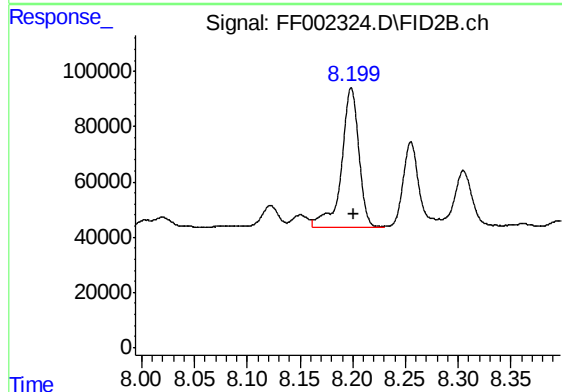


#4 N-TETRADECANE

R.T.: 8.199 min
Delta R.T.: -0.002 min
Response: 574754
Conc: 3.45 ug/ml

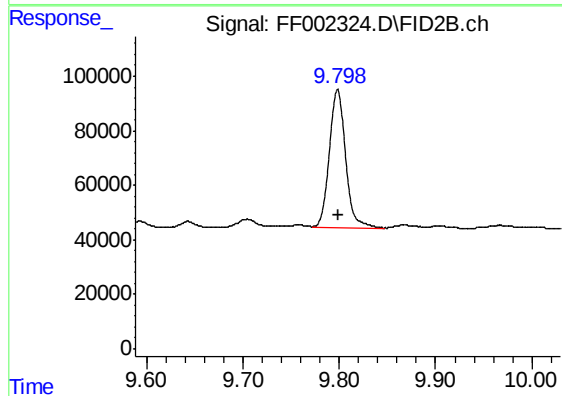


#5 N-HEXADECANE

R.T.: 9.798 min
Delta R.T.: 0.000 min
Response: 585829
Conc: 3.50 ug/ml m

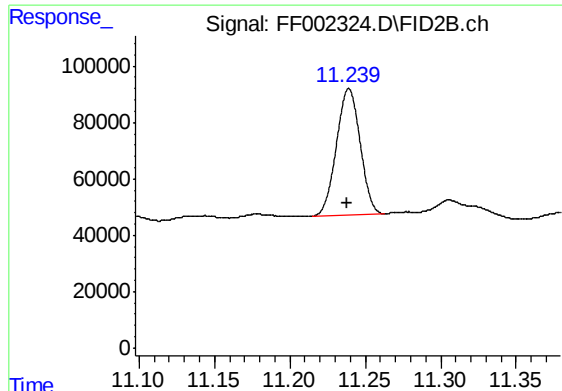


#6 N-OCTADECANE

R.T.: 11.239 min
Delta R.T.: 0.000 min
Response: 491248
Conc: 2.93 ug/ml m

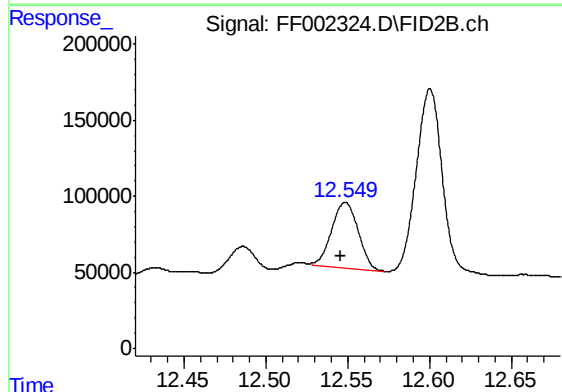


#7 N-EICOSANE

R.T.: 12.549 min
Delta R.T.: 0.003 min
Response: 482169
Conc: 2.91 ug/ml m

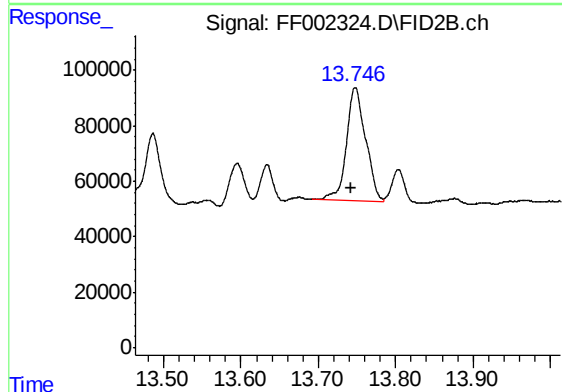


#8 N-DOCOSANE

R.T.: 13.748 min
Delta R.T.: 0.005 min
Response: 703848
Conc: 4.31 ug/ml

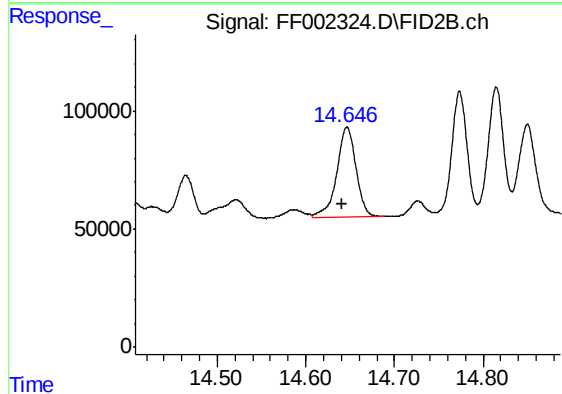


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.646 min
Delta R.T.: 0.006 min
Response: 569641
Conc: 3.99 ug/ml

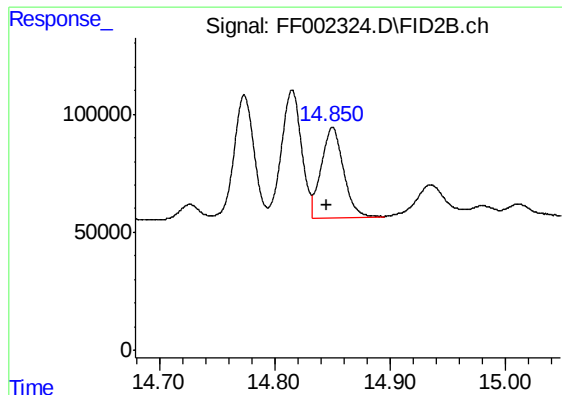


#10 N-TETRACOSANE

R.T.: 14.850 min
Delta R.T.: 0.006 min
Response: 514046
Conc: 3.21 ug/ml

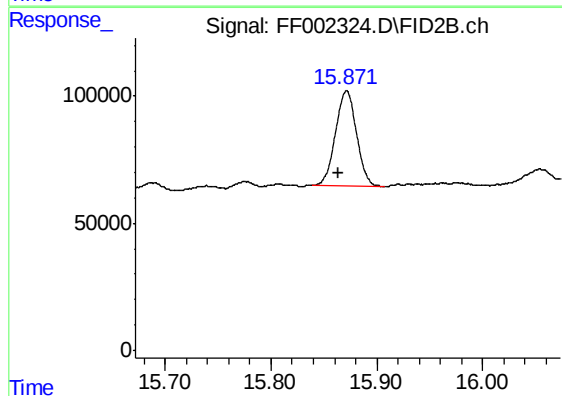

#11 N-HEXACOSANE

R.T.: 15.871 min
Delta R.T.: 0.007 min
Response: 519309
Conc: 3.32 ug/ml m

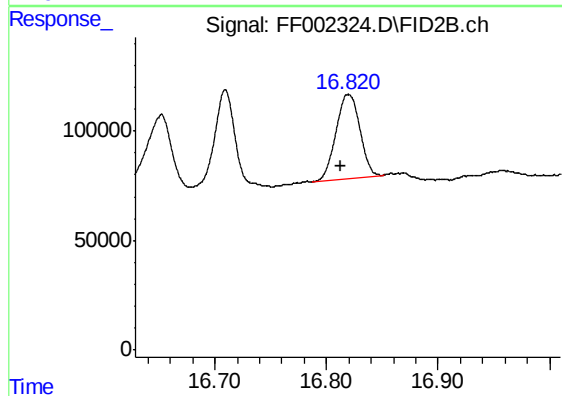

#12 N-OCTACOSANE

R.T.: 16.820 min
Delta R.T.: 0.007 min
Response: 572759
Conc: 3.74 ug/ml m