

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100319\
 Data File : FF005724.D
 Signal(s) : FID2B.ch
 Acq On : 03 Oct 2019 15:01
 Operator : DD\AJ
 Sample : K4839-19 5X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RR-DIES-WP

Integration File: autoint1.e
 Quant Time: Oct 04 01:23:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
 Quant Title :
 QLast Update : Thu Oct 03 04:07:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.673	527003	4.053 ug/ml
Target Compounds			
2) N-DECANE	4.418	1189173	7.658 ug/ml
3) N-DODECANE	6.436	1808868	11.486 ug/ml
4) N-TETRADECANE	8.229	2142170	13.631 ug/ml
5) N-HEXADECANE	9.829	1983320	12.582 ug/ml
6) N-OCTADECANE	11.269	1456007	9.384 ug/ml
7) N-EICOSANE	12.578	803697	5.191 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100319\
Data File : FF005724.D
Signal(s) : FID2B.ch
Acq On : 03 Oct 2019 15:01
Operator : DD\AJ
Sample : K4839-19 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Oct 04 01:23:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
Quant Title :
QLast Update : Thu Oct 03 04:07:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

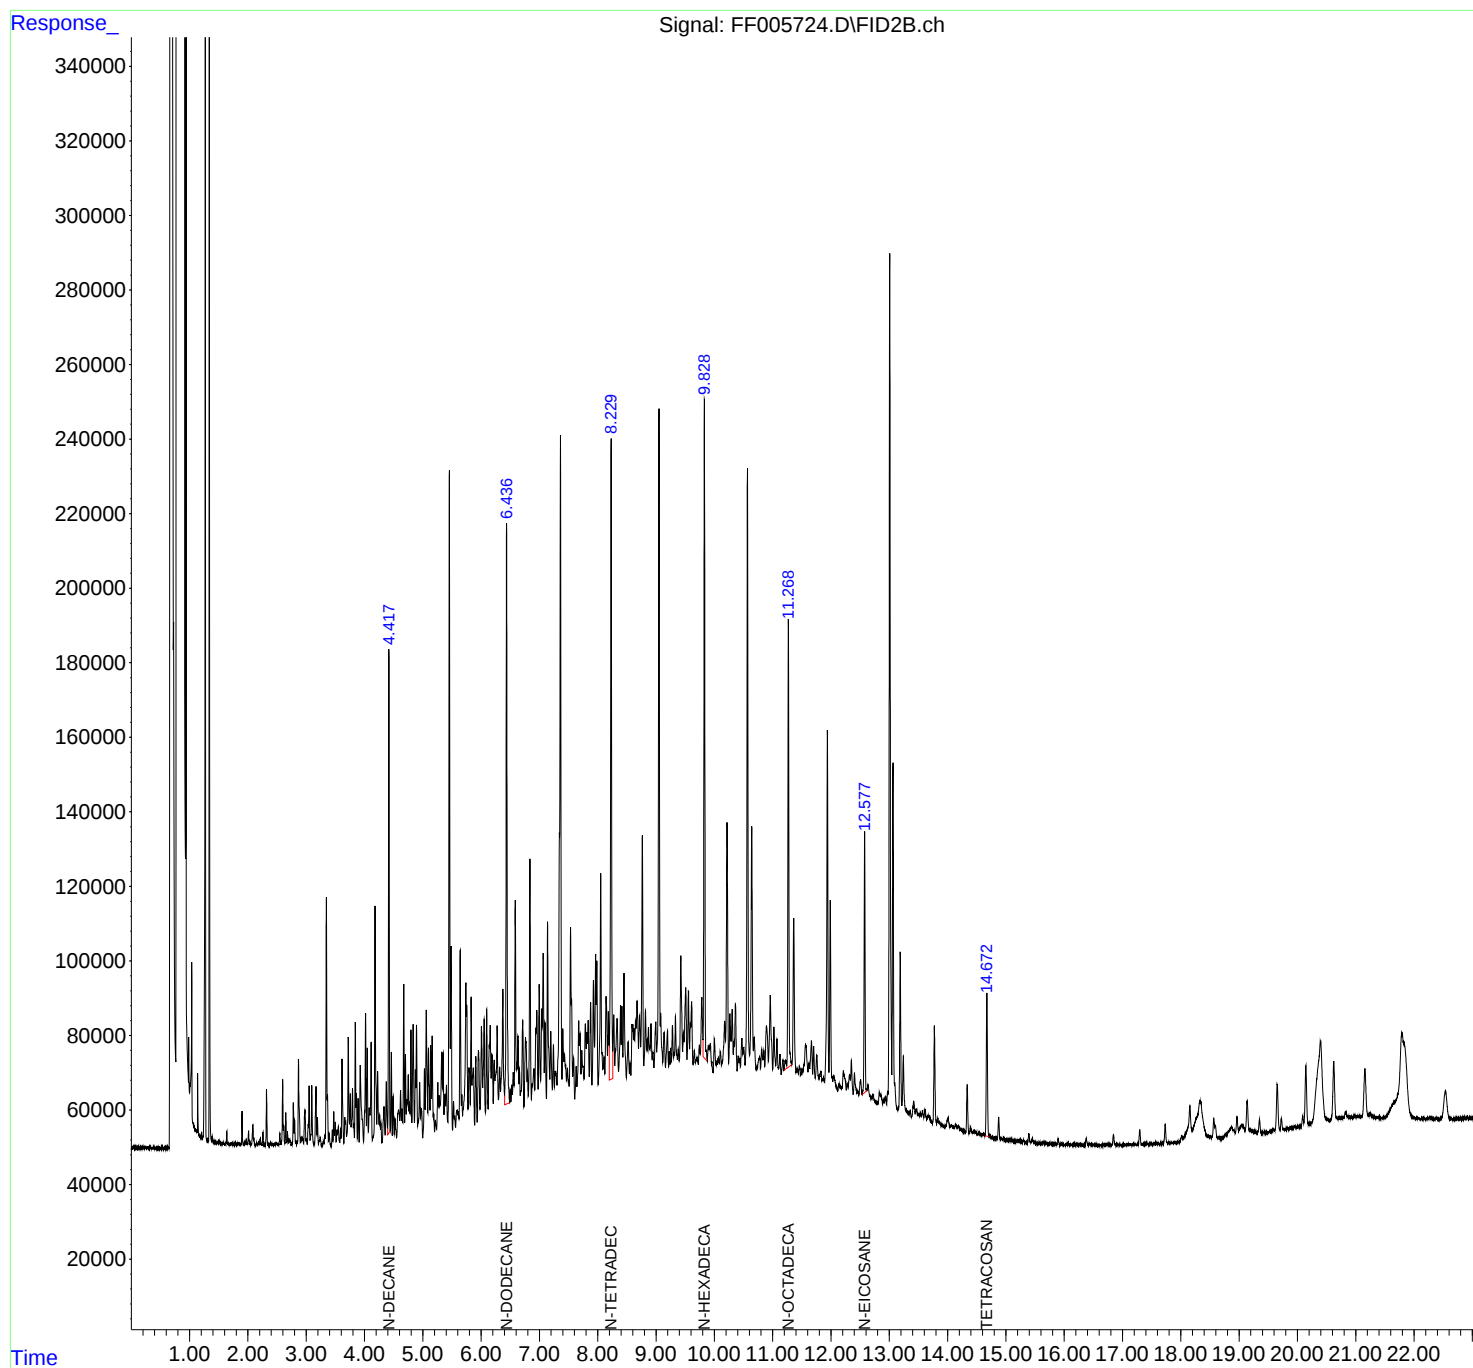


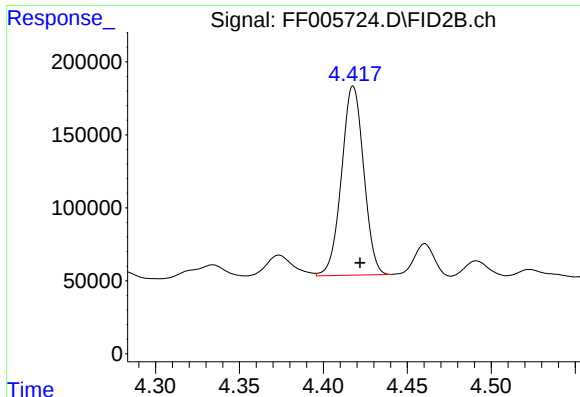

#2 N-DECANE


R.T.: 4.418 min
Delta R.T.: -0.004 min
Response: 1189173
Conc: 7.66 ug/ml

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

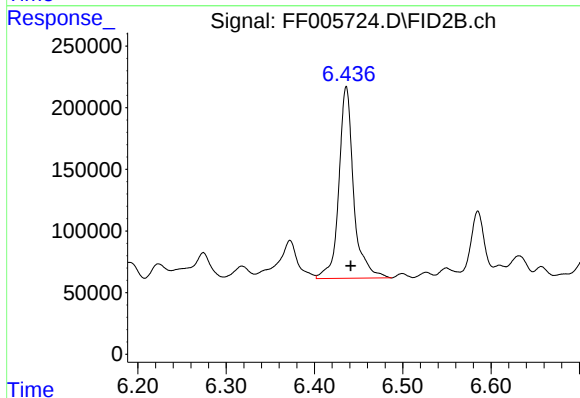


#3 N-DODECANE

R.T.: 6.436 min
Delta R.T.: -0.005 min
Response: 1808868
Conc: 11.49 ug/ml

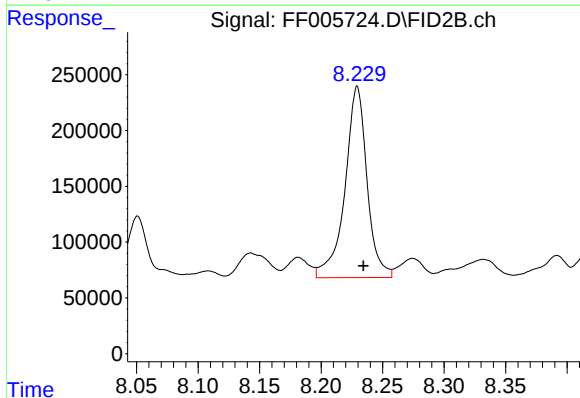


#4 N-TETRADECANE

R.T.: 8.229 min
Delta R.T.: -0.005 min
Response: 2142170
Conc: 13.63 ug/ml

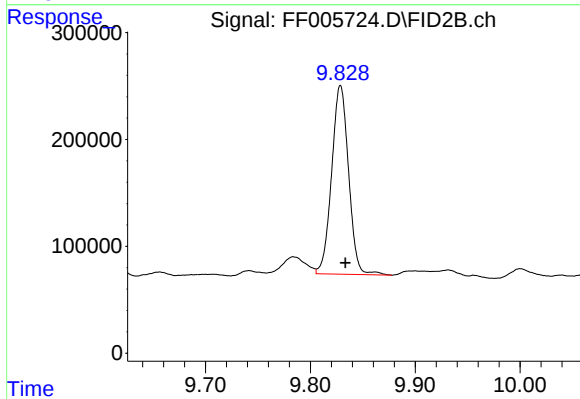

#5 N-HEXADECANE


R.T.: 9.829 min
Delta R.T.: -0.005 min
Response: 1983320
Conc: 12.58 ug/ml

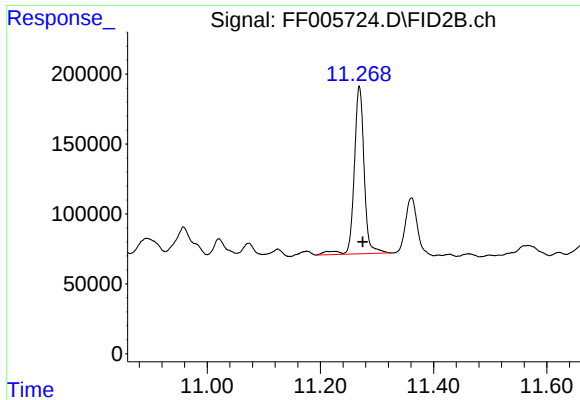

#6 N-OCTADECANE


R.T.: 11.269 min
Delta R.T.: -0.006 min
Response: 1456007
Conc: 9.38 ug/ml

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

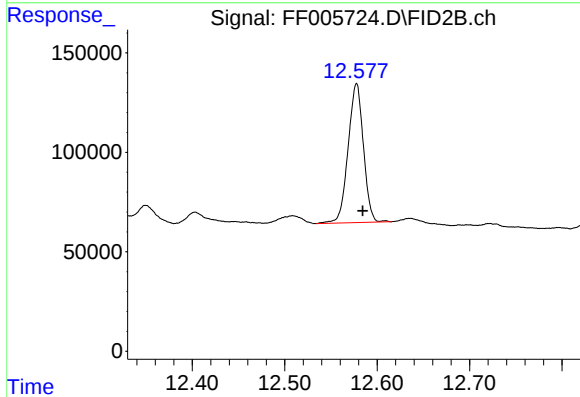

#7 N-EICOSANE

R.T.: 12.578 min
Delta R.T.: -0.007 min
Response: 803697
Conc: 5.19 ug/ml

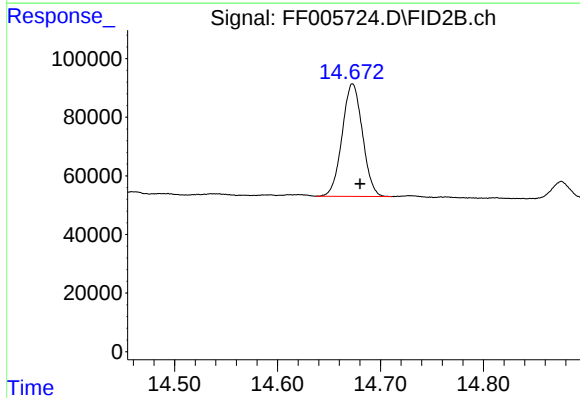

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.673 min
Delta R.T.: -0.007 min
Response: 527003
Conc: 4.05 ug/ml