Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100319\
Data File : FF005725.D
Signal(s) : FID2B.ch
Acq On : 03 Oct 2019 15:30
Operator : DD\AJ
Sample : K4839-19 10X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 04 01:23:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
Quant Title :
QLast Update : Thu Oct 03 04:07:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units
	System Monitoring Compounds			
	Target Compounds			
2)	N-DECANE	4.420	604804	3.895 ug/ml
3)	N-DODECANE	6.438	896208	5.691 ug/ml
4)	N-TETRADECANE	8.230	982315	6.250 ug/ml
5)	N-HEXADECANE	9.830	1020205	6.472 ug/ml
6)	N-OCTADECANE	11.269	676854	4.363 ug/ml
7)	N-EICOSANE	12.577	411008	2.655 ug/ml

(f)=RT Delta > 1/2 Window (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100319\
Data File : FF005725.D
Signal(s) : FID2B.ch
Acq On : 03 Oct 2019 15:30
Operator : DD\AJ
Sample : K4839-19 10X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 04 01:23:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
Quant Title :
QLast Update : Thu Oct 03 04:07:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

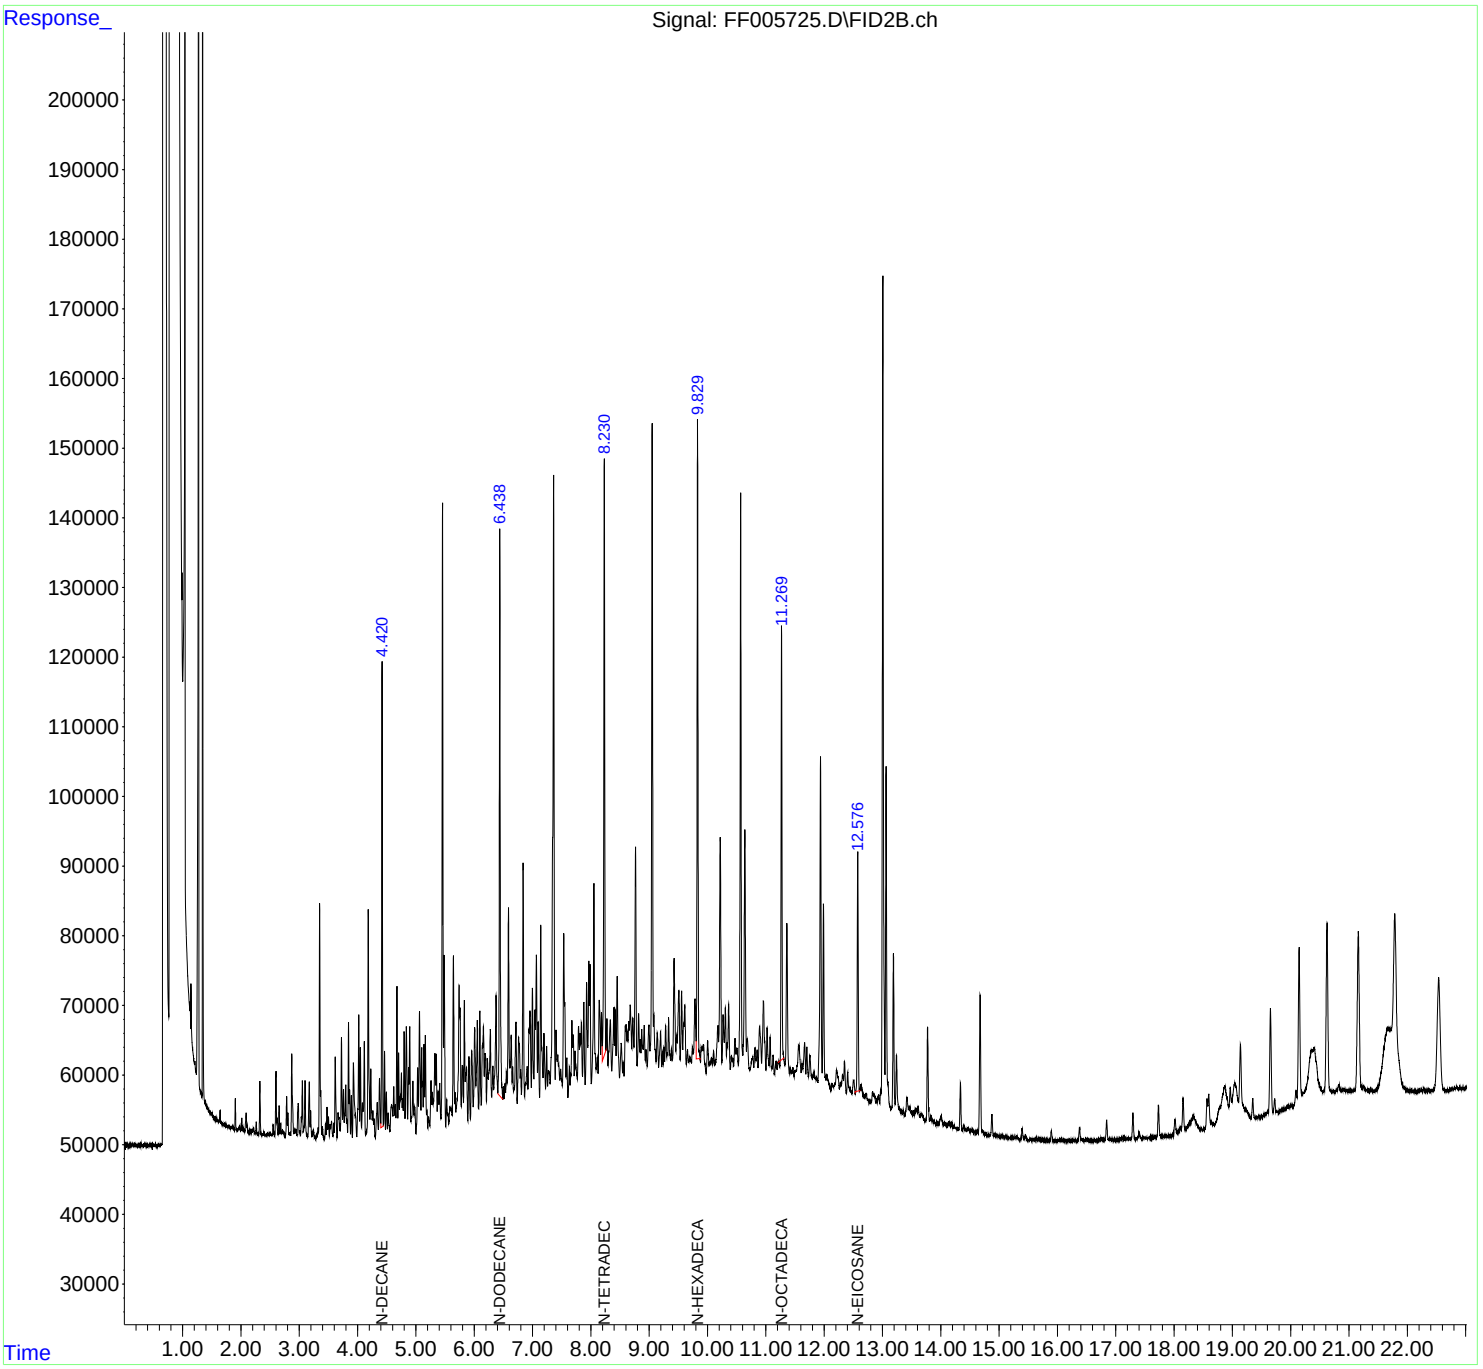

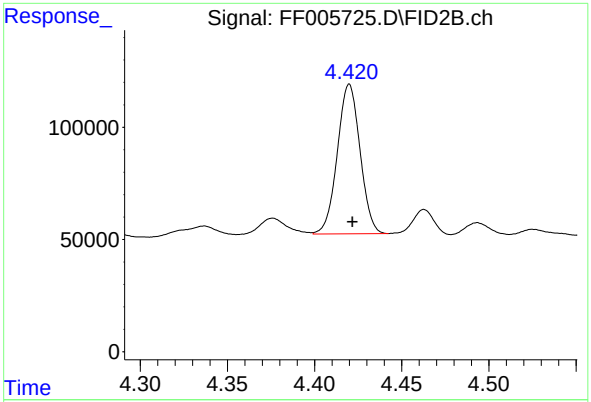

#2 N-DECANE

R.T.: 4.420 min
Delta R.T.: -0.002 min
Response: 604804
Conc: 3.89 ug/ml

Instrument :
FID_F
ClientSampleId :

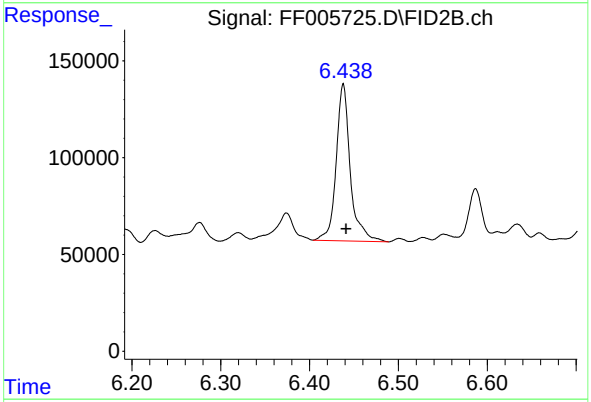

#3 N-DODECANE

R.T.: 6.438 min
Delta R.T.: -0.003 min
Response: 896208
Conc: 5.69 ug/ml

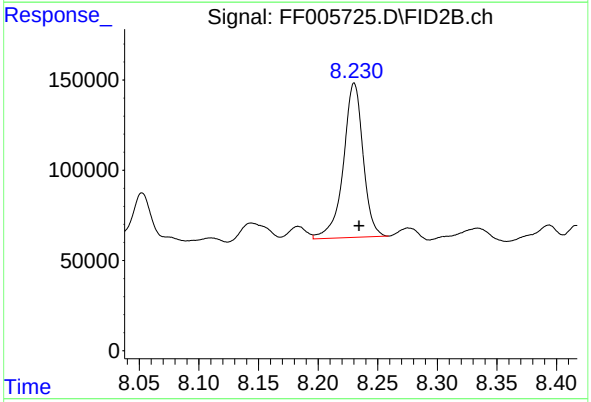

#4 N-TETRADECANE

R.T.: 8.230 min
Delta R.T.: -0.004 min
Response: 982315
Conc: 6.25 ug/ml

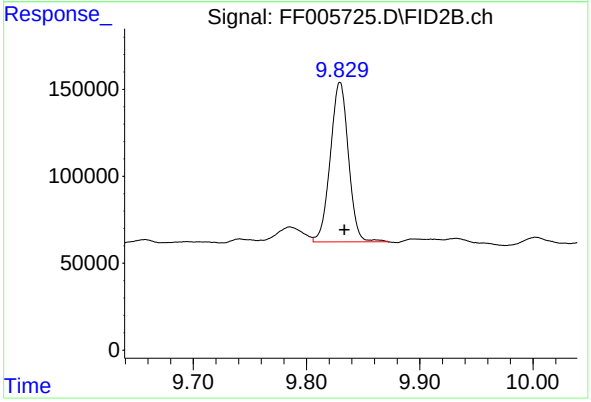

#5 N-HEXADECANE

R.T.: 9.830 min
Delta R.T.: -0.004 min
Response: 1020205
Conc: 6.47 ug/ml

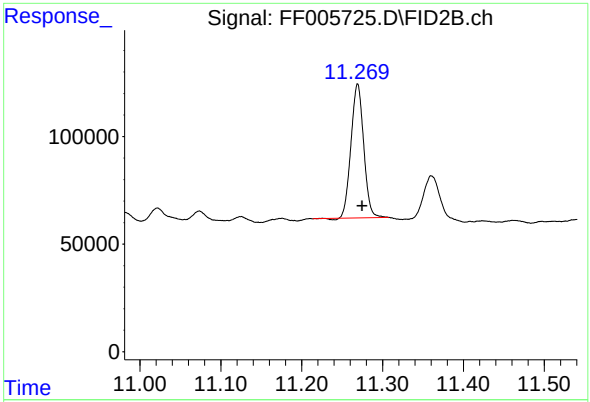

#6 N-OCTADECANE

R.T.: 11.269 min
Delta R.T.: -0.005 min
Response: 676854
Conc: 4.36 ug/ml

Instrument :
FID_F
ClientSampleId :

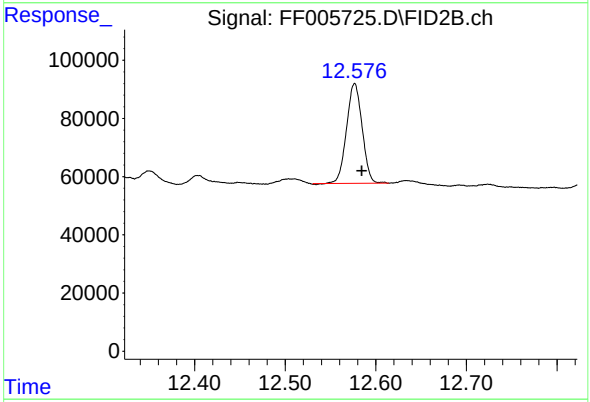

#7 N-EICOSANE

R.T.: 12.577 min
Delta R.T.: -0.008 min
Response: 411008
Conc: 2.65 ug/ml

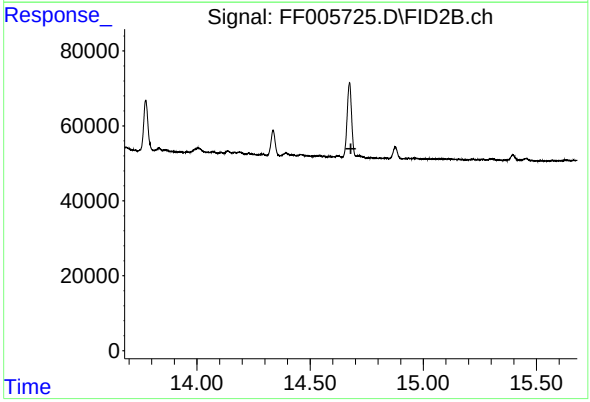

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.680 min
Response: 0
Conc: N.D.