

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100523\
 Data File : FF013516.D
 Signal(s) : FID2B.ch
 Acq On : 05 Oct 2023 08:59
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 05 23:54:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
 Quant Title :
 QLast Update : Thu Sep 21 15:19:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.004	294751	2.618 ug/ml
Target Compounds			
12) N-OCTACOSANE	17.139	54328	0.466 ug/ml
13) N-TRIACONTANE	18.027	84609	0.735 ug/ml
14) N-DOTRIACONTANE	18.859	109392	0.941 ug/ml
16) N-HEXATRIACONTANE	20.431	64408	0.861 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100523\
Data File : FF013516.D
Signal(s) : FID2B.ch
Acq On : 05 Oct 2023 08:59
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 05 23:54:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

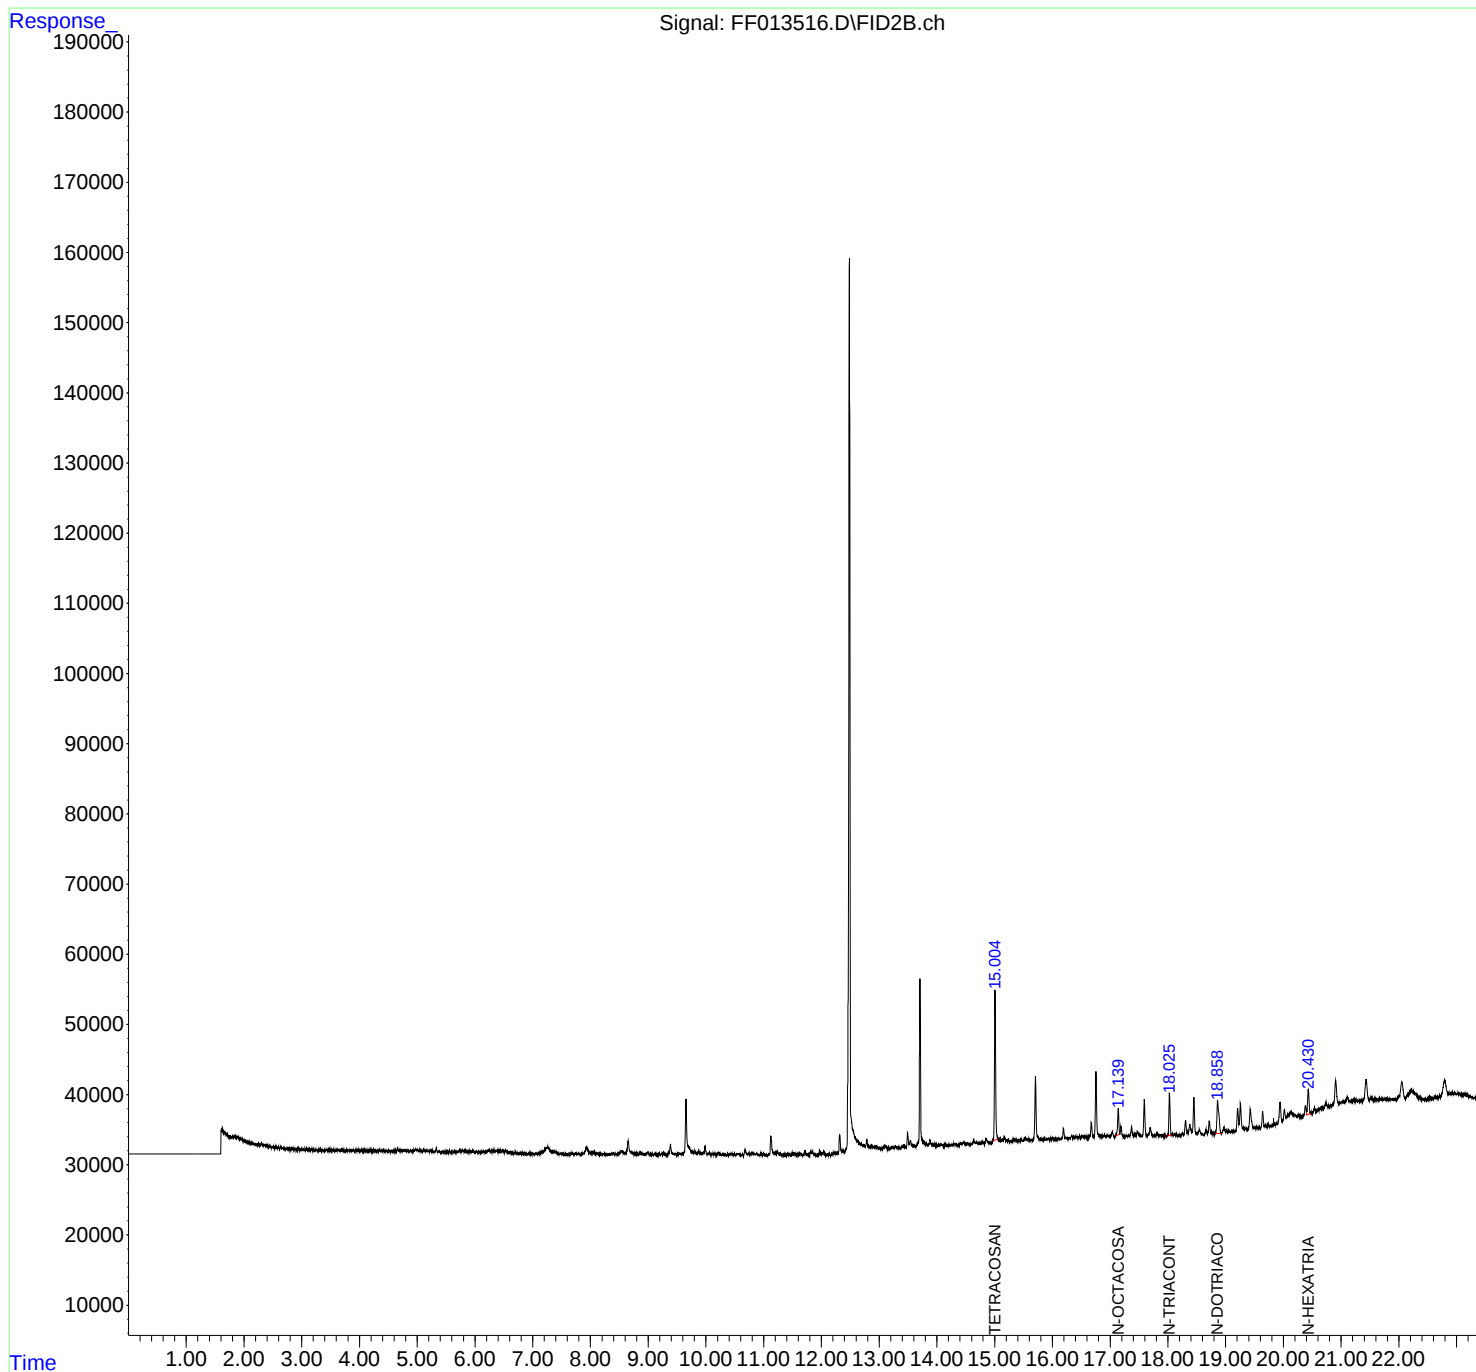


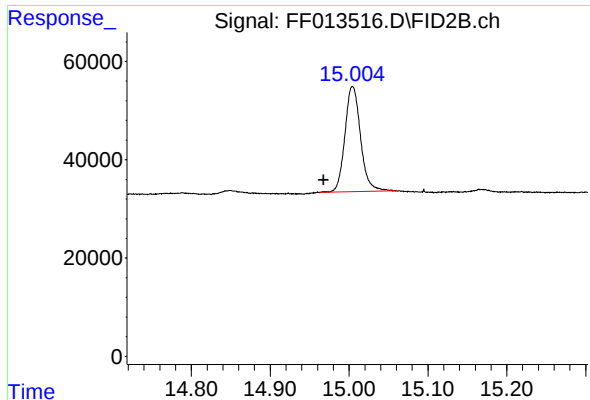

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.004 min
Delta R.T.: 0.037 min
Response: 294751
Conc: 2.62 ug/ml

Instrument :
FID_F
ClientSampleId :

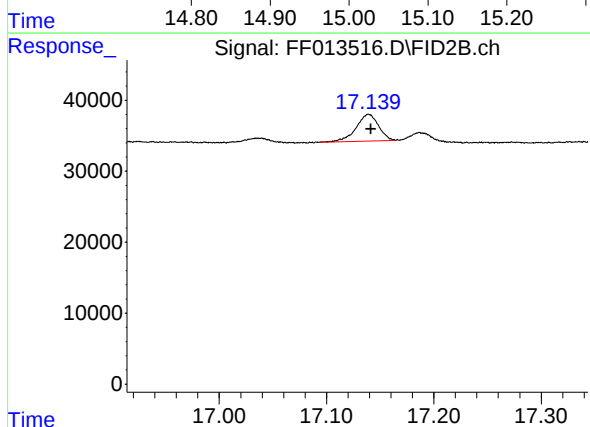


#12 N-OCTACOSANE

R.T.: 17.139 min
Delta R.T.: -0.002 min
Response: 54328
Conc: 0.47 ug/ml

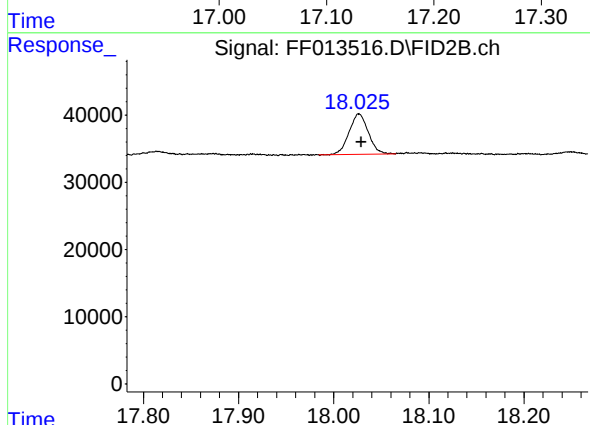


#13 N-TRIACONTANE

R.T.: 18.027 min
Delta R.T.: -0.003 min
Response: 84609
Conc: 0.74 ug/ml

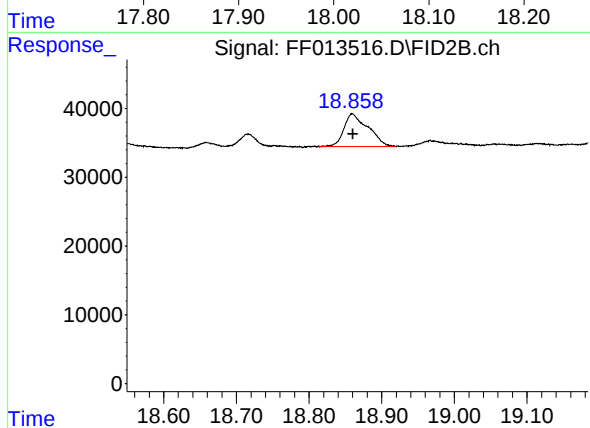

#14 N-DOTRIACONTANE

R.T.: 18.859 min
Delta R.T.: -0.001 min
Response: 109392
Conc: 0.94 ug/ml

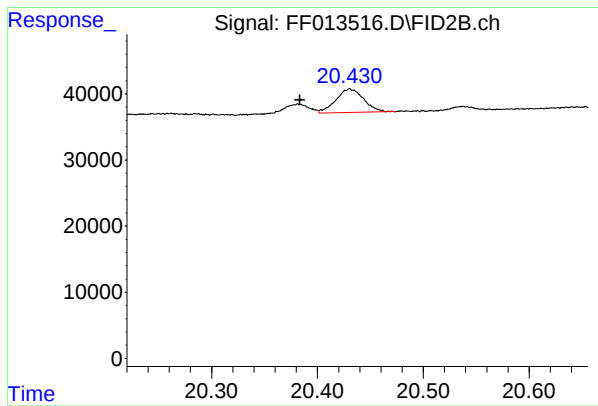

#16 N-HEXATRIACONTANE

R.T.: 20.431 min
Delta R.T.: 0.047 min
Response: 64408
Conc: 0.86 ug/ml

Instrument :

FID_F

ClientSampleId :