

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100523\
 Data File : FF013520.D
 Signal(s) : FID2B.ch
 Acq On : 05 Oct 2023 12:27
 Operator : YP\AJ
 Sample : PB156107BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 05 23:55:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
 Quant Title :
 QLast Update : Thu Sep 21 15:19:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.967	2327453	20.673 ug/ml
Target Compounds			
12) N-OCTACOSANE	17.139	47549	0.408 ug/ml
13) N-TRIACONTANE	18.026	130603	1.135 ug/ml
14) N-DOTRIACONTANE	18.858	184475	1.587 ug/ml
15) N-TETRATRIACONTANE	19.641	132250	1.414 ug/ml
16) N-HEXATRIACONTANE	20.381	83780	1.120 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100523\
Data File : FF013520.D
Signal(s) : FID2B.ch
Acq On : 05 Oct 2023 12:27
Operator : YP\AJ
Sample : PB156107BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 05 23:55:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

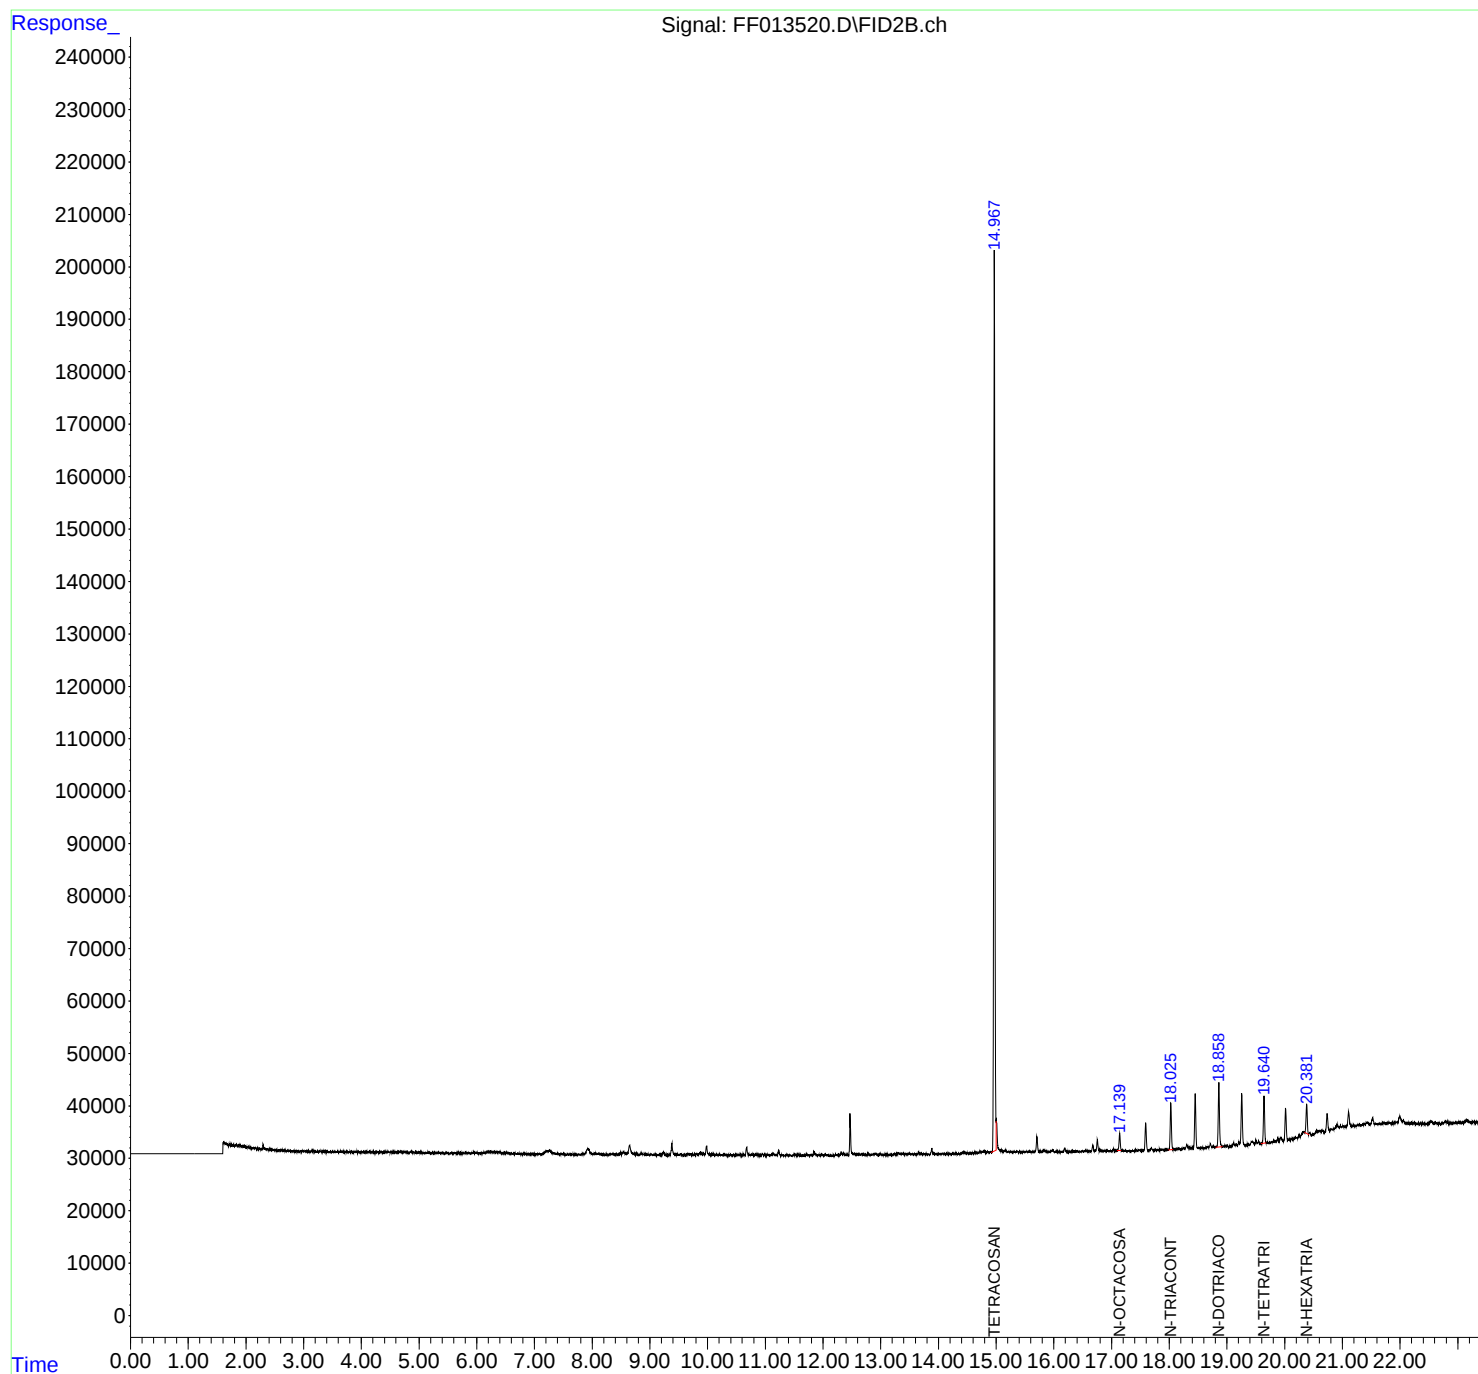


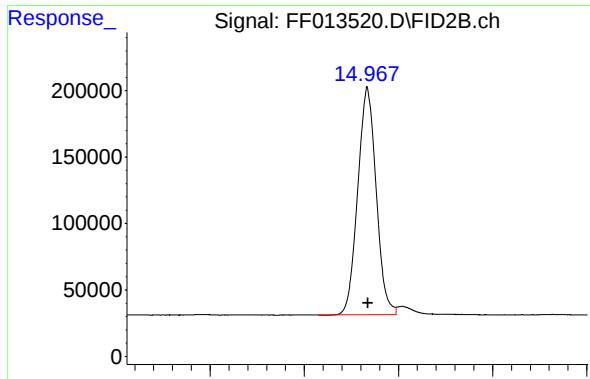

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.967 min
Delta R.T.: 0.000 min
Response: 2327453
Conc: 20.67 ug/ml

Instrument :
FID_F
ClientSampleId :

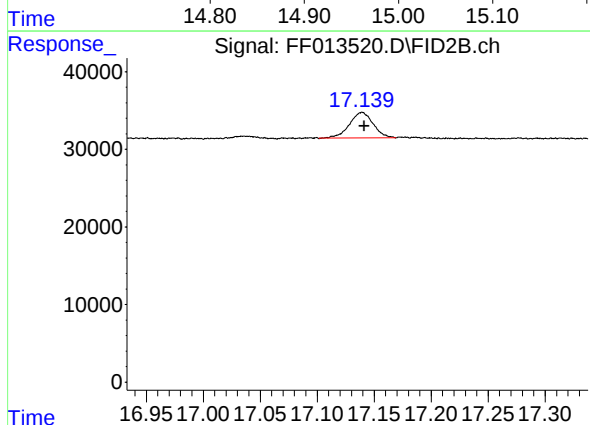


#12 N-OCTACOSANE

R.T.: 17.139 min
Delta R.T.: -0.002 min
Response: 47549
Conc: 0.41 ug/ml

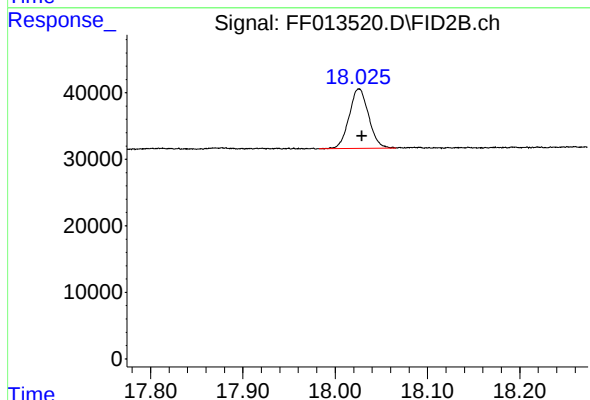


#13 N-TRIACONTANE

R.T.: 18.026 min
Delta R.T.: -0.003 min
Response: 130603
Conc: 1.13 ug/ml

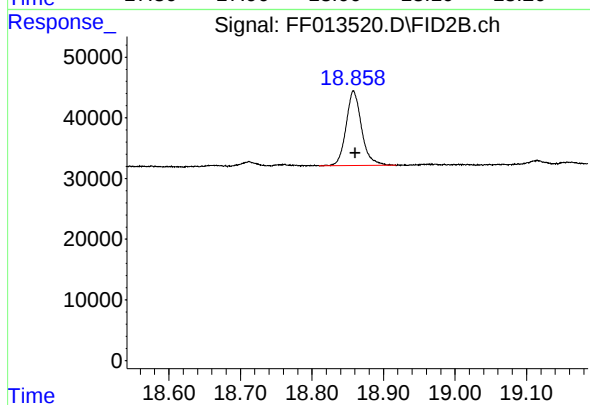

#14 N-DOTRIACONTANE


R.T.: 18.858 min
Delta R.T.: -0.002 min
Response: 184475
Conc: 1.59 ug/ml

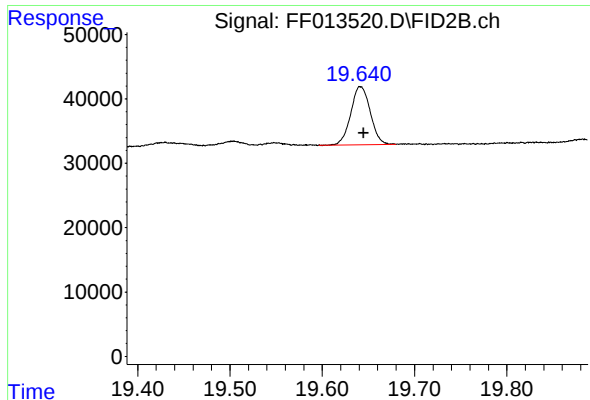

#15 N-TETRATRIACONTANE

R.T.: 19.641 min
Delta R.T.: -0.003 min
Response: 132250
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :

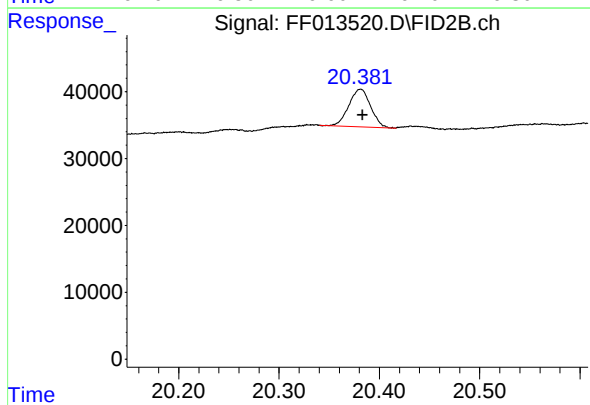

#16 N-HEXATRIACONTANE

R.T.: 20.381 min
Delta R.T.: -0.002 min
Response: 83780
Conc: 1.12 ug/ml