

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100523\
Data File : FF013531.D
Signal(s) : FID2B.ch
Acq On : 05 Oct 2023 17:53
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 05 23:57:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.967	2128486	18.906 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.881	77235	0.664 ug/ml
16) N-HEXATRIACONTANE	20.433	73887	0.988 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100523\
Data File : FF013531.D
Signal(s) : FID2B.ch
Acq On : 05 Oct 2023 17:53
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 05 23:57:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

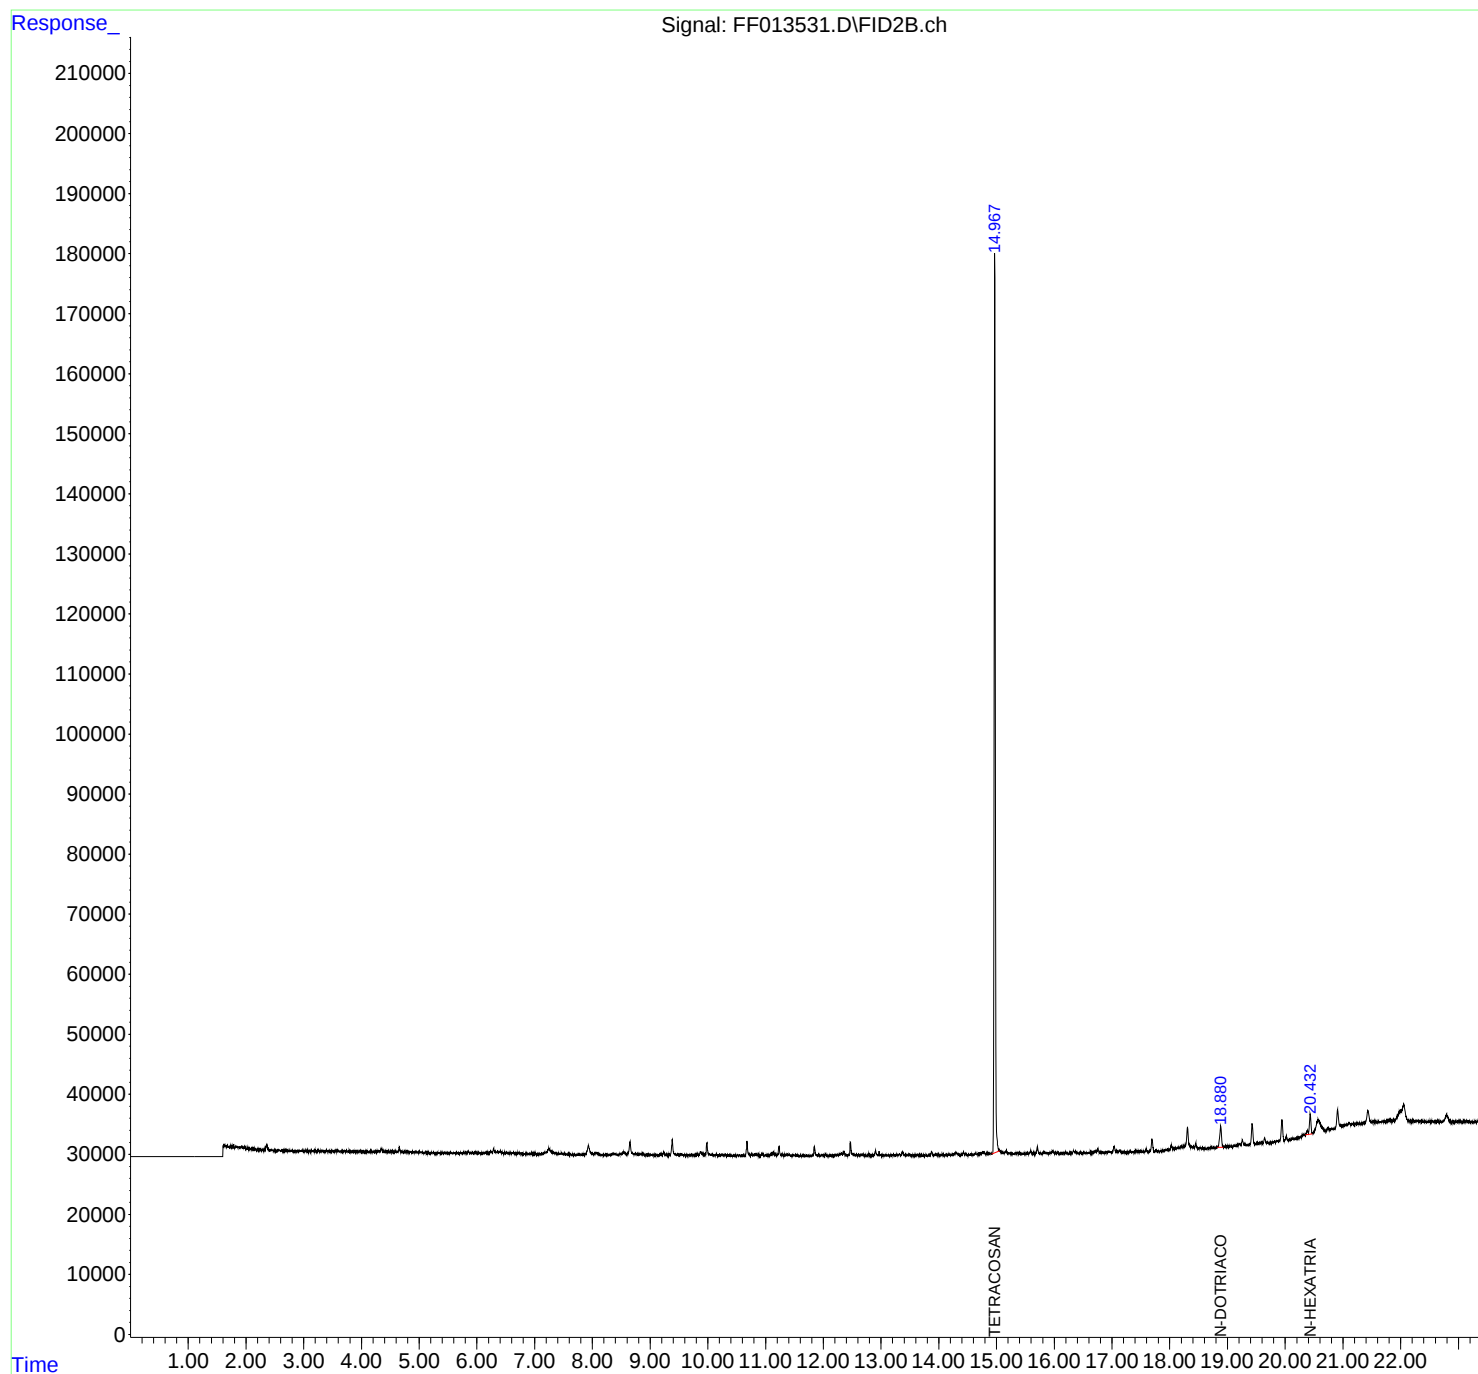


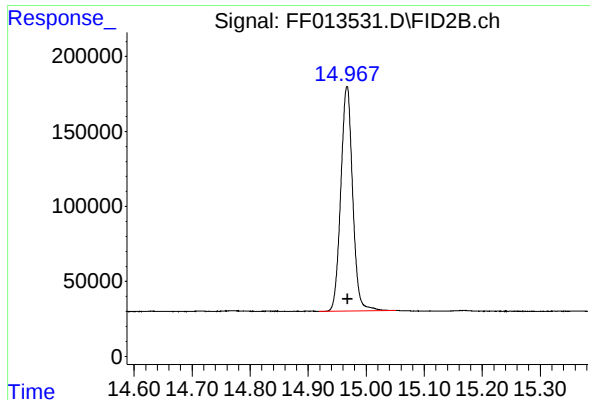

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.967 min
Delta R.T.: 0.000 min
Response: 2128486
Conc: 18.91 ug/ml

Instrument : FID_F
ClientSampleId :

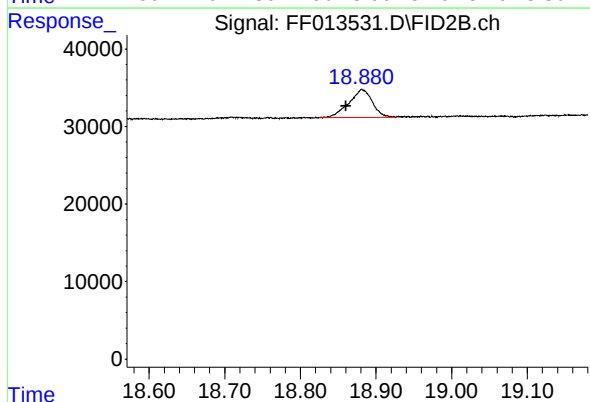

#14 N-DOTRIACONTANE

R.T.: 18.881 min
Delta R.T.: 0.021 min
Response: 77235
Conc: 0.66 ug/ml

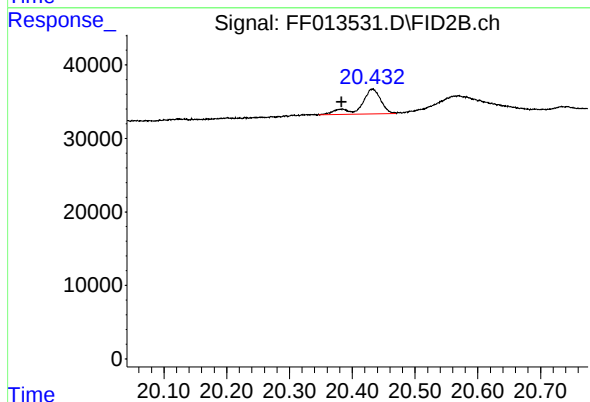

#16 N-HEXATRIACONTANE

R.T.: 20.433 min
Delta R.T.: 0.049 min
Response: 73887
Conc: 0.99 ug/ml