

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100523\
 Data File : FF013544.D
 Signal(s) : FID2B.ch
 Acq On : 06 Oct 2023 02:16
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 06 04:12:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
 Quant Title :
 QLast Update : Thu Sep 21 15:19:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.967	2127956	18.901 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.883	95070	0.818 ug/ml
16) N-HEXATRIACONTANE	20.434f	66587	0.890 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100523\
Data File : FF013544.D
Signal(s) : FID2B.ch
Acq On : 06 Oct 2023 02:16
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 06 04:12:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

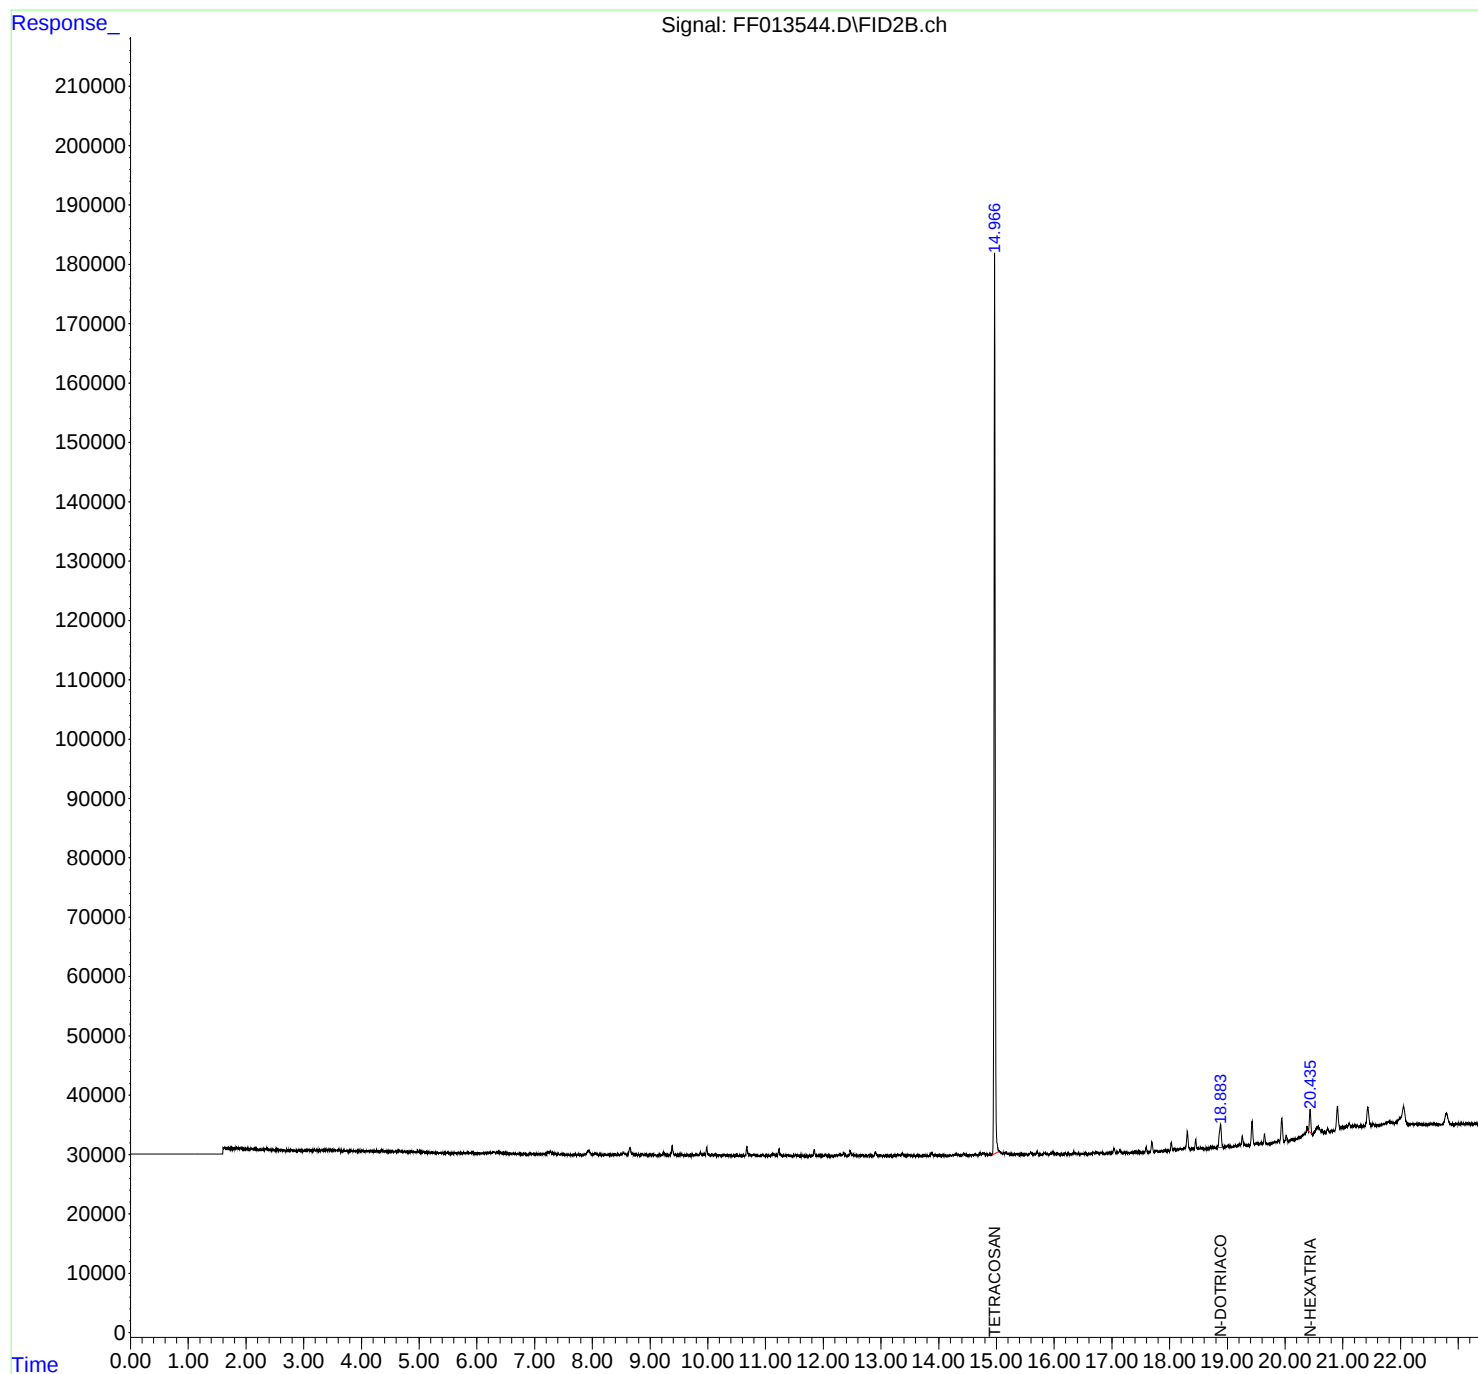

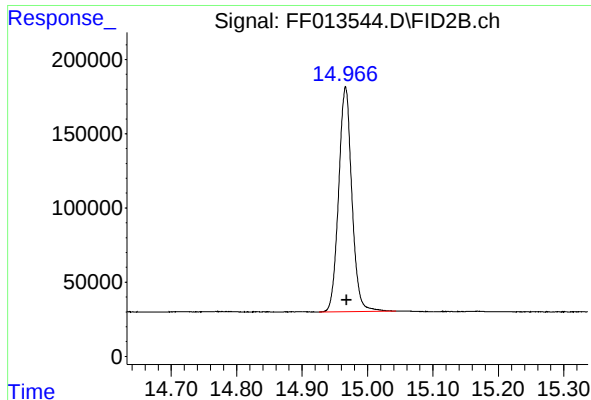


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.967 min
Delta R.T.: -0.001 min
Response: 2127956
Conc: 18.90 ug/ml

Instrument :


FID_F

ClientSampleId :

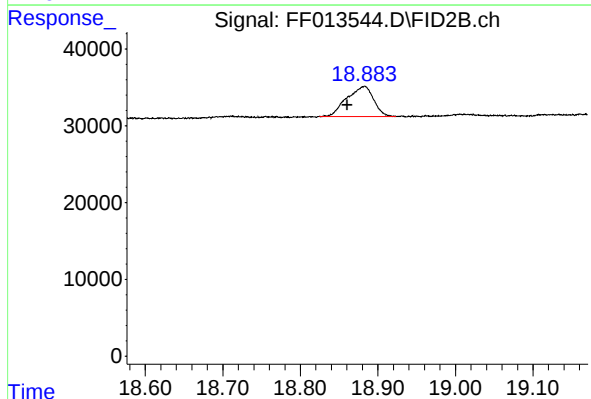

#14 N-DOTRIACONTANE

R.T.: 18.883 min
Delta R.T.: 0.022 min
Response: 95070
Conc: 0.82 ug/ml

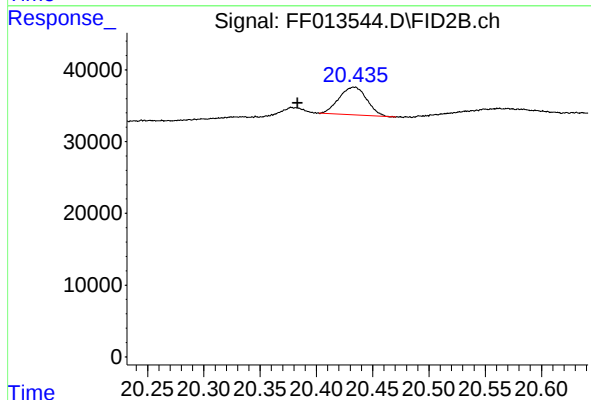

#16 N-HEXATRIACONTANE

R.T.: 20.434 min
Delta R.T.: 0.050 min
Response: 66587
Conc: 0.89 ug/ml