

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100623\
Data File : FF013551.D
Signal(s) : FID2B.ch
Acq On : 06 Oct 2023 09:25
Operator : YP\AJ
Sample : PB156131BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 07 01:47:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.966	2321514	20.620 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.026	48259	0.419 ug/ml
14) N-DOTRIACONTANE	18.861	104253	0.897 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100623\
Data File : FF013551.D
Signal(s) : FID2B.ch
Acq On : 06 Oct 2023 09:25
Operator : YP\AJ
Sample : PB156131BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 07 01:47:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

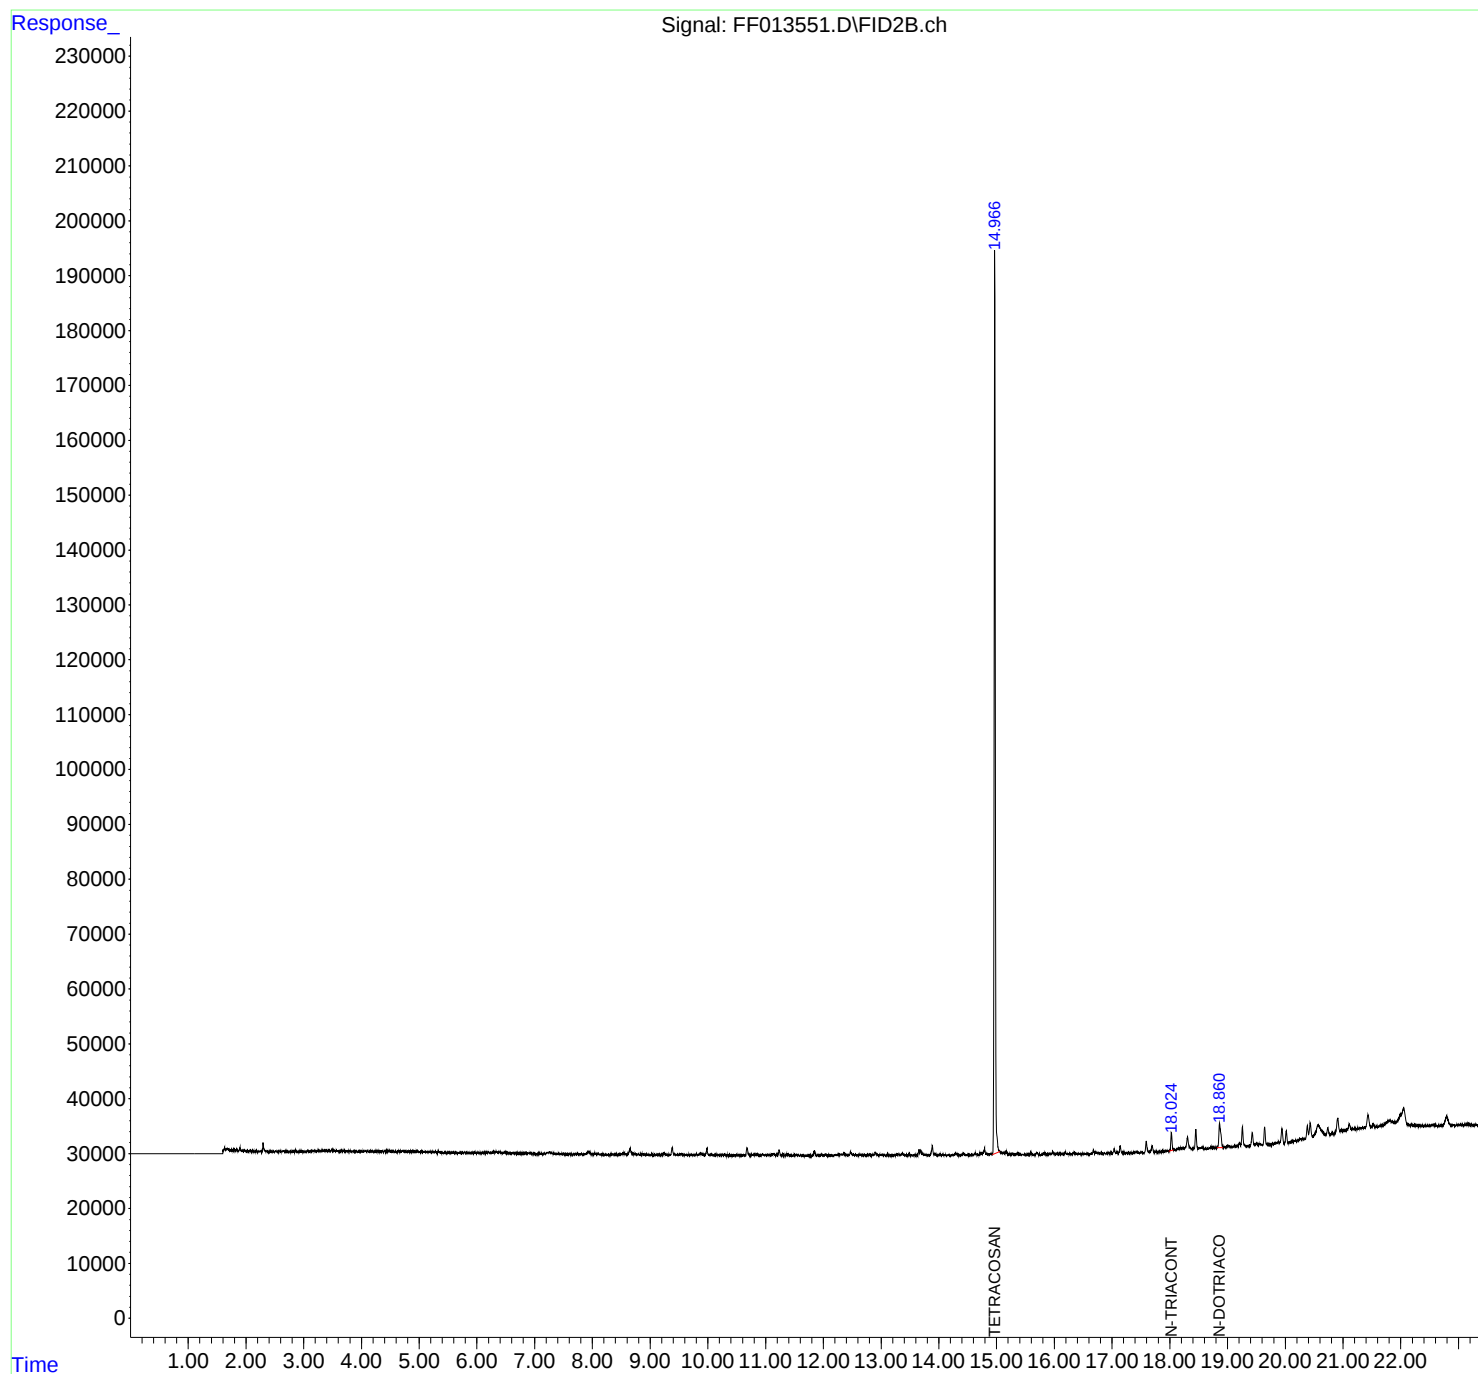

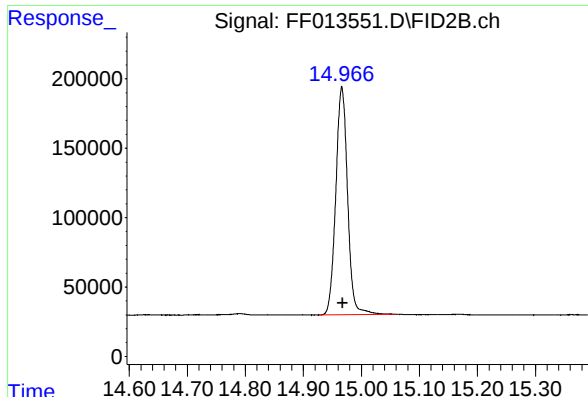


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.966 min
Delta R.T.: -0.002 min
Response: 2321514
Conc: 20.62 ug/ml

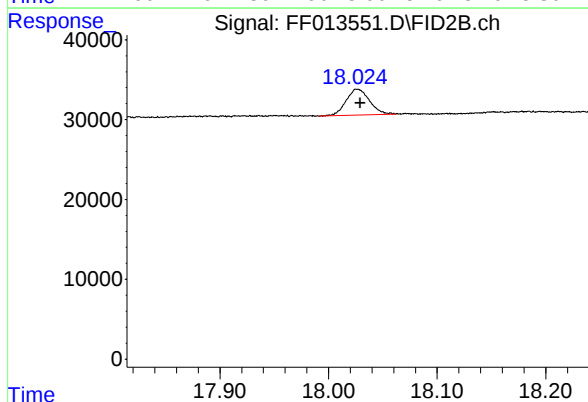

#13 N-TRIACONTANE

R.T.: 18.026 min
Delta R.T.: -0.003 min
Response: 48259
Conc: 0.42 ug/ml

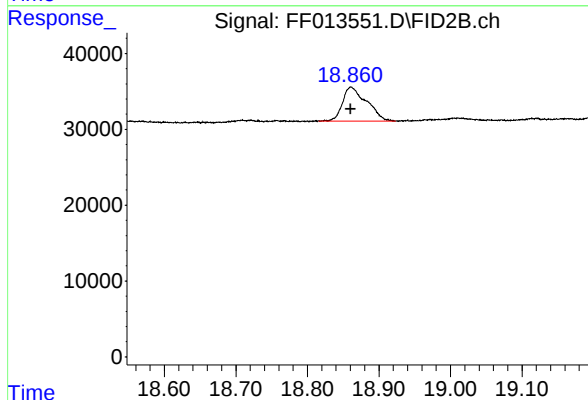

#14 N-DOTRIACONTANE

R.T.: 18.861 min
Delta R.T.: 0.000 min
Response: 104253
Conc: 0.90 ug/ml