

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100623\
Data File : FF013560.D
Signal(s) : FID2B.ch
Acq On : 06 Oct 2023 14:28
Operator : YP\AJ
Sample : PB156111BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 07 01:48:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.969	2230925	19.815 ug/ml
Target Compounds				
13)	N-TRIACONTANE	18.030	47268	0.411 ug/ml
14)	N-DOTRIACONTANE	18.863	100566	0.865 ug/ml
15)	N-TETRATRIACONTANE	19.644	49588	0.530 ug/ml
18)	N-TETRACONTANE	22.058f	137176	1.940 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100623\
Data File : FF013560.D
Signal(s) : FID2B.ch
Acq On : 06 Oct 2023 14:28
Operator : YP\AJ
Sample : PB156111BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 07 01:48:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

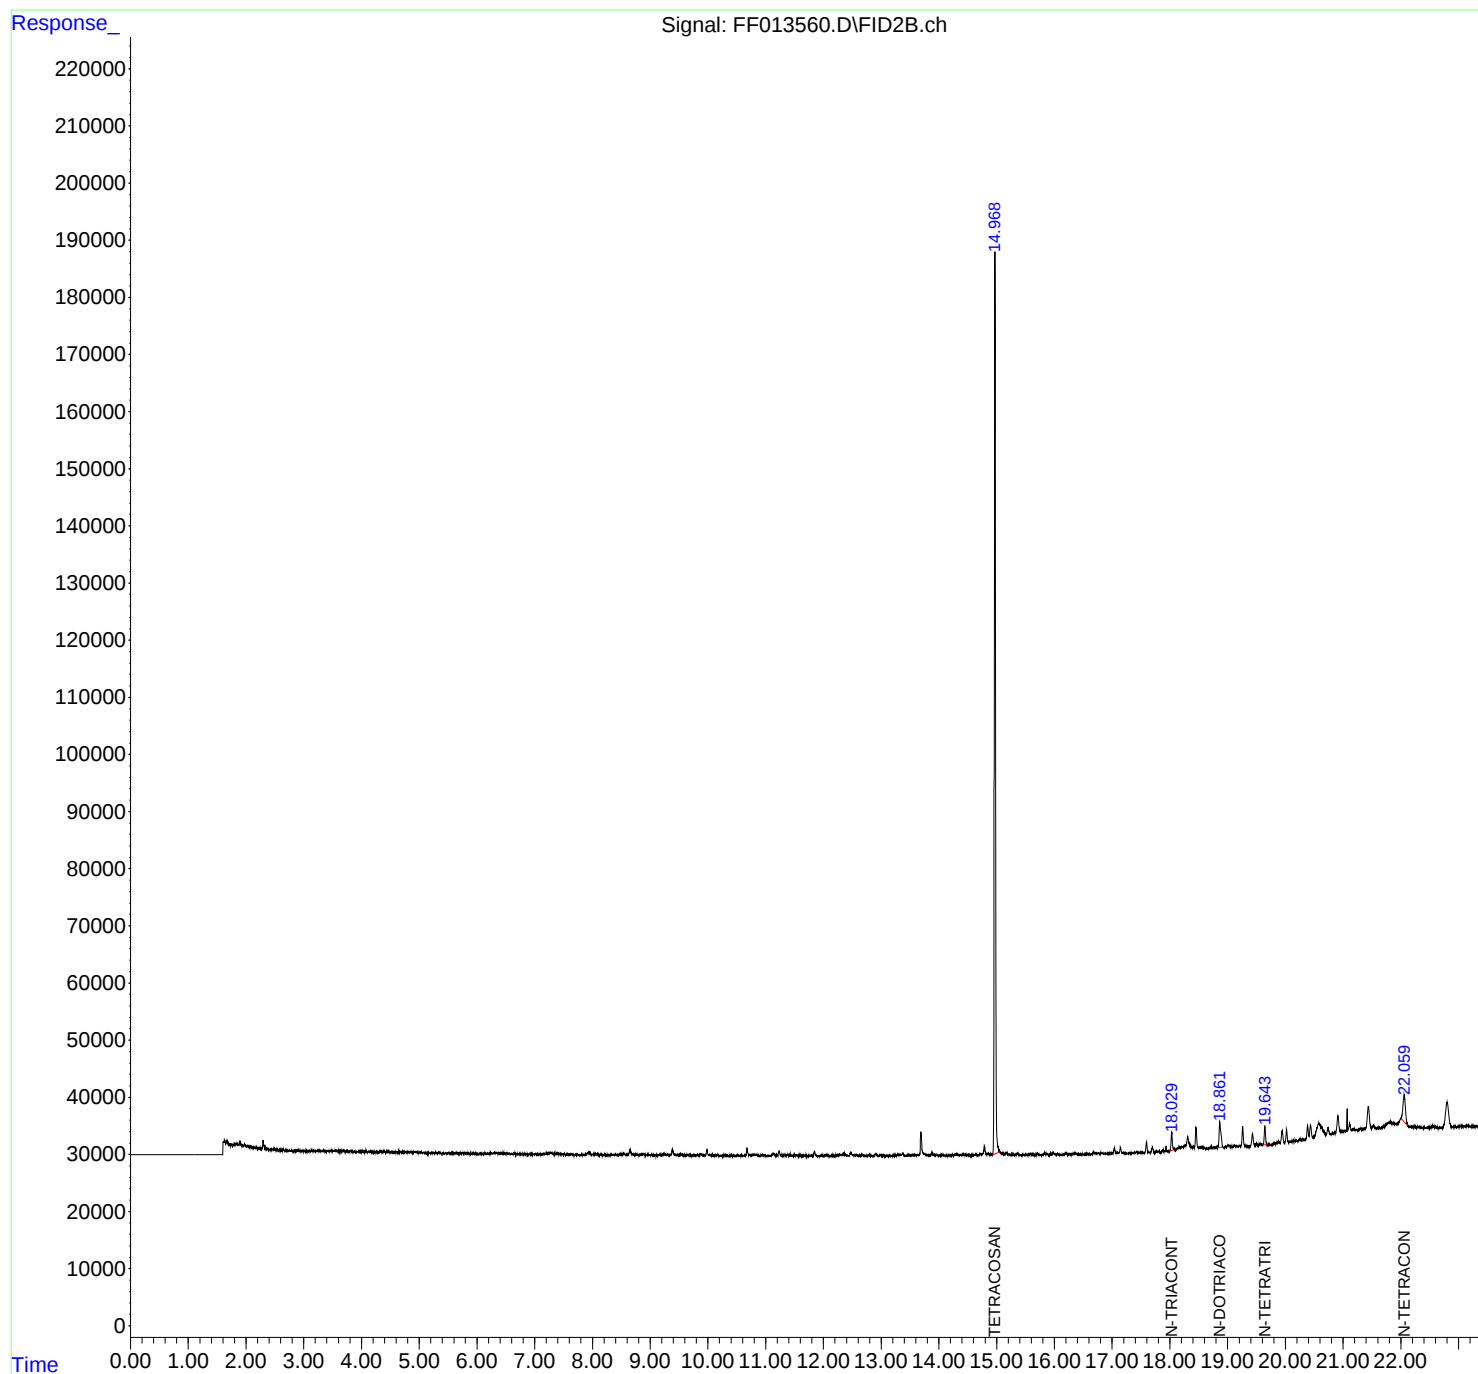

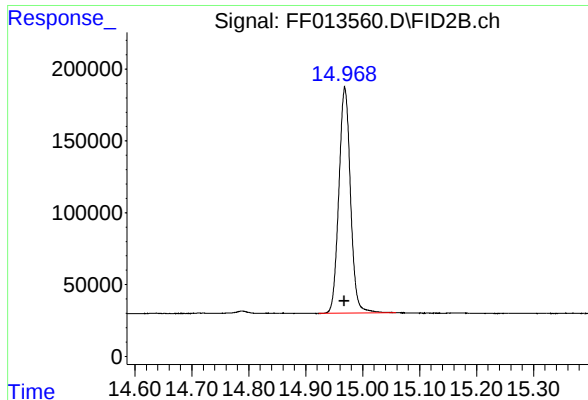


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.969 min
Delta R.T.: 0.000 min
Response: 2230925
Conc: 19.82 ug/ml

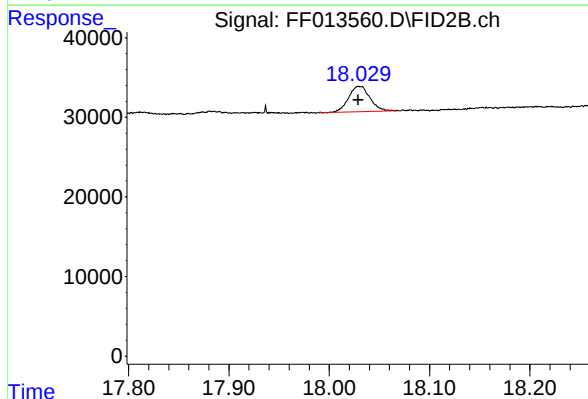


#13 N-TRIACONTANE

R.T.: 18.030 min
Delta R.T.: 0.000 min
Response: 47268
Conc: 0.41 ug/ml

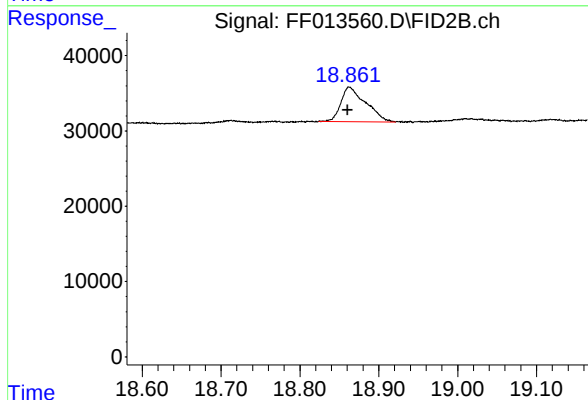


#14 N-DOTRIACONTANE

R.T.: 18.863 min
Delta R.T.: 0.002 min
Response: 100566
Conc: 0.87 ug/ml

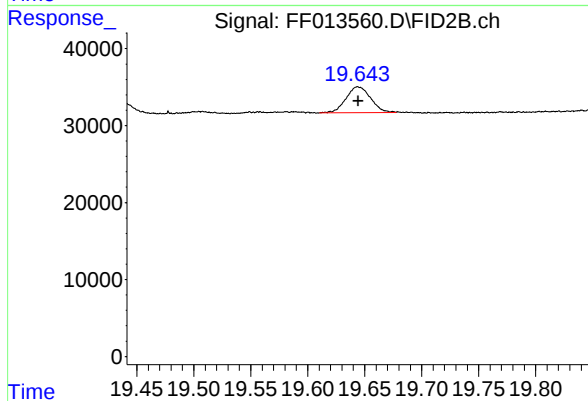

#15 N-TETRATRIACONTANE

R.T.: 19.644 min
Delta R.T.: 0.000 min
Response: 49588
Conc: 0.53 ug/ml

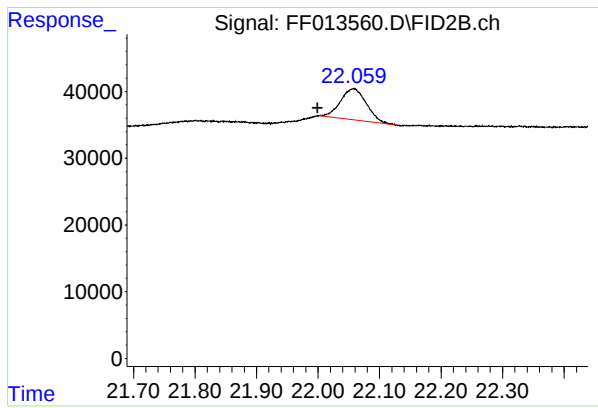

#18 N-TETRACONTANE

R.T.: 22.058 min
Delta R.T.: 0.059 min
Response: 137176
Conc: 1.94 ug/ml