

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100623\
Data File : FF013563.D
Signal(s) : FID2B.ch
Acq On : 06 Oct 2023 15:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 07 01:49:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.969	1853789	16.466 ug/ml

Target Compounds


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100623\
Data File : FF013563.D
Signal(s) : FID2B.ch
Acq On : 06 Oct 2023 15:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 07 01:49:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF092123.M
Quant Title :
QLast Update : Thu Sep 21 15:19:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

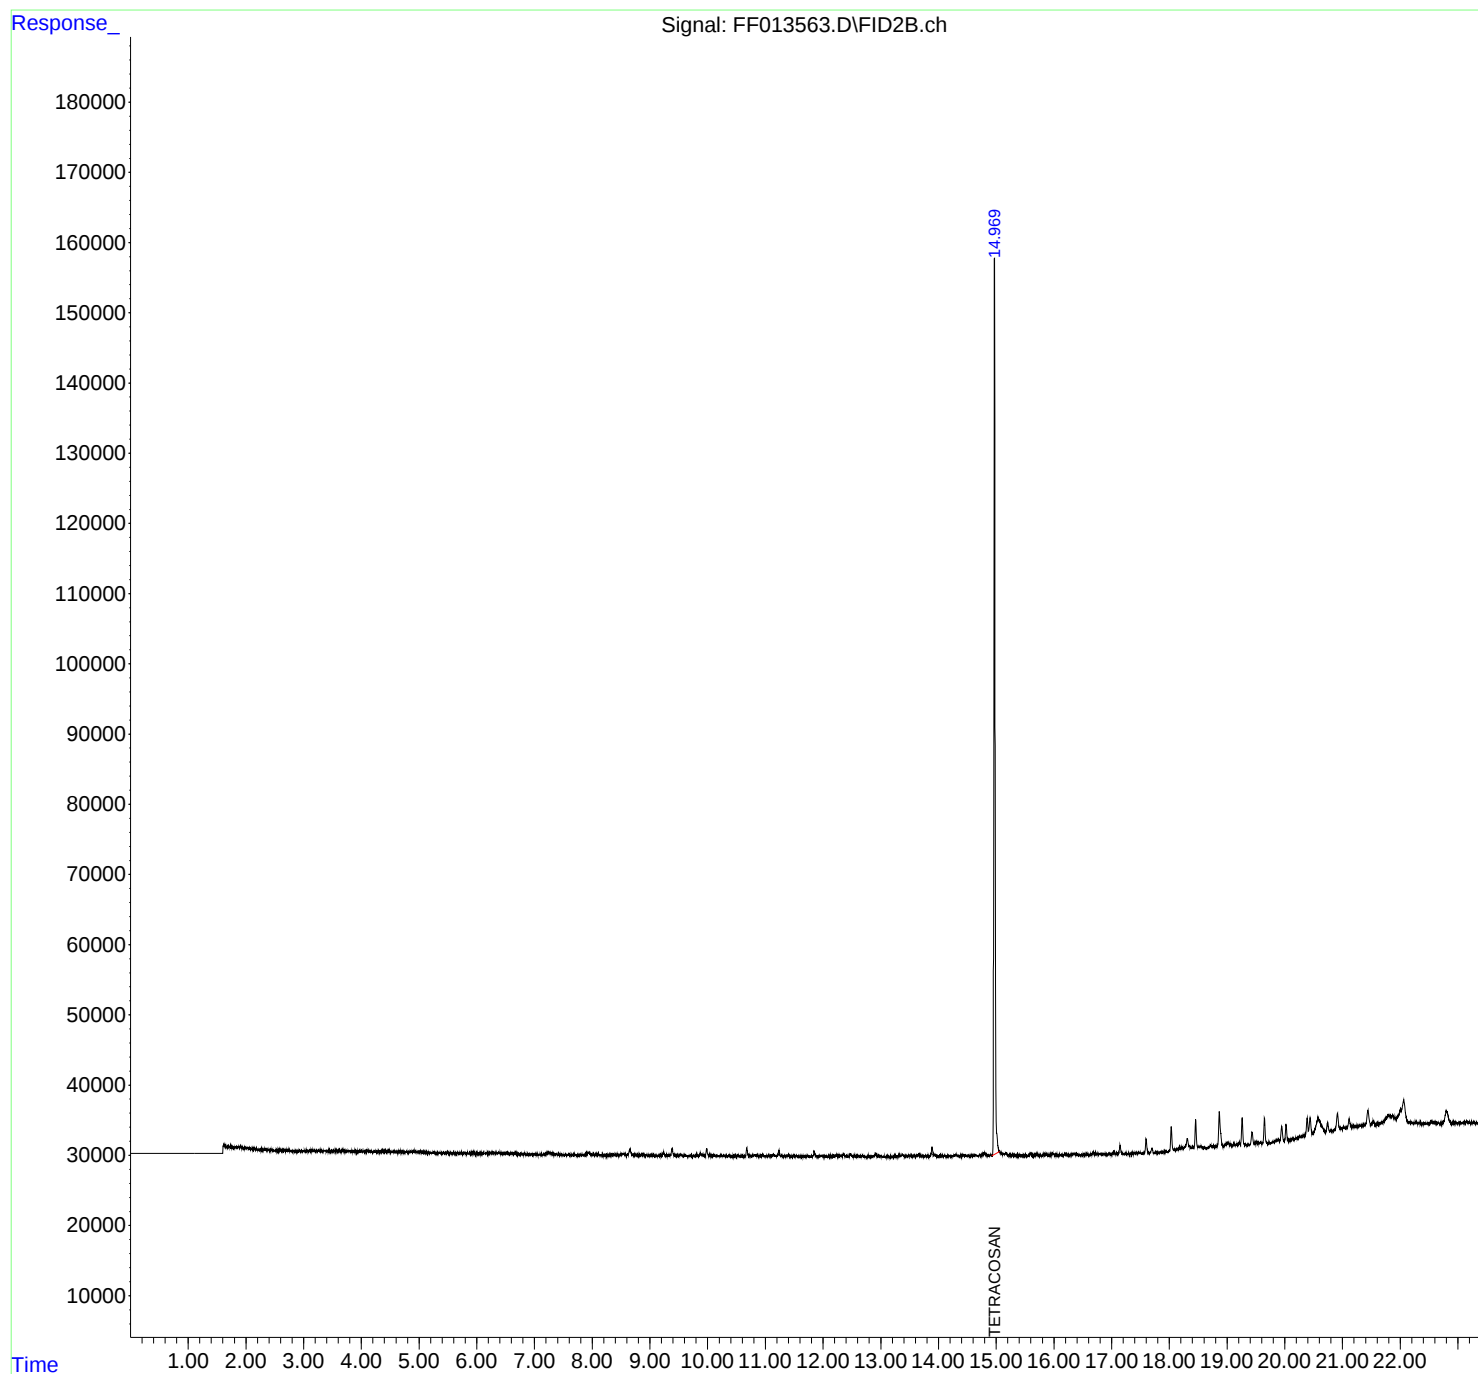

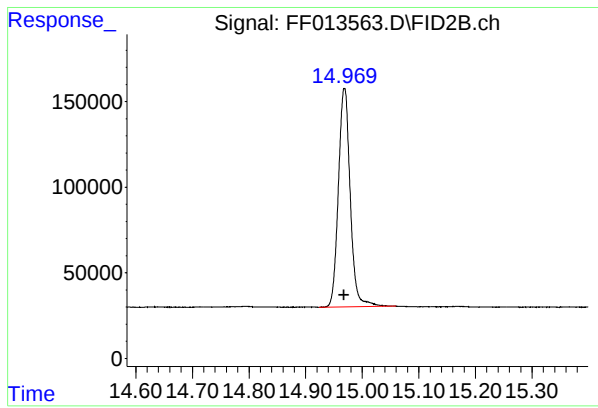

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.969 min
Delta R.T.: 0.000 min
Response: 1853789
Conc: 16.47 ug/ml