

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100819\
 Data File : FF005745.D
 Signal(s) : FID2B.ch
 Acq On : 08 Oct 2019 15:44
 Operator : DD\AJ
 Sample : PB123731BS
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Oct 09 01:22:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
 Quant Title :
 QLast Update : Thu Oct 03 04:07:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.670	2401183	18.467 ug/ml
Target Compounds			
2) N-DECANE	4.419	3139333	20.217 ug/ml
3) N-DODECANE	6.437	3161749	20.077 ug/ml
4) N-TETRADECANE	8.229	3118036	19.840 ug/ml
5) N-HEXADECANE	9.827	3086049	19.577 ug/ml
6) N-OCTADECANE	11.267	2990307	19.274 ug/ml
7) N-EICOSANE	12.574	2932282	18.939 ug/ml
8) N-DOCOSANE	13.771	2825337	18.617 ug/ml
10) N-TETRACOSANE	14.873	2723863	18.306 ug/ml
11) N-HEXACOSANE	15.892	2625915	17.999 ug/ml
12) N-OCTACOSANE	16.841	2525824	17.735 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100819\
Data File : FF005745.D
Signal(s) : FID2B.ch
Acq On : 08 Oct 2019 15:44
Operator : DD\AJ
Sample : PB123731BS
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Oct 09 01:22:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
Quant Title :
QLast Update : Thu Oct 03 04:07:51 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

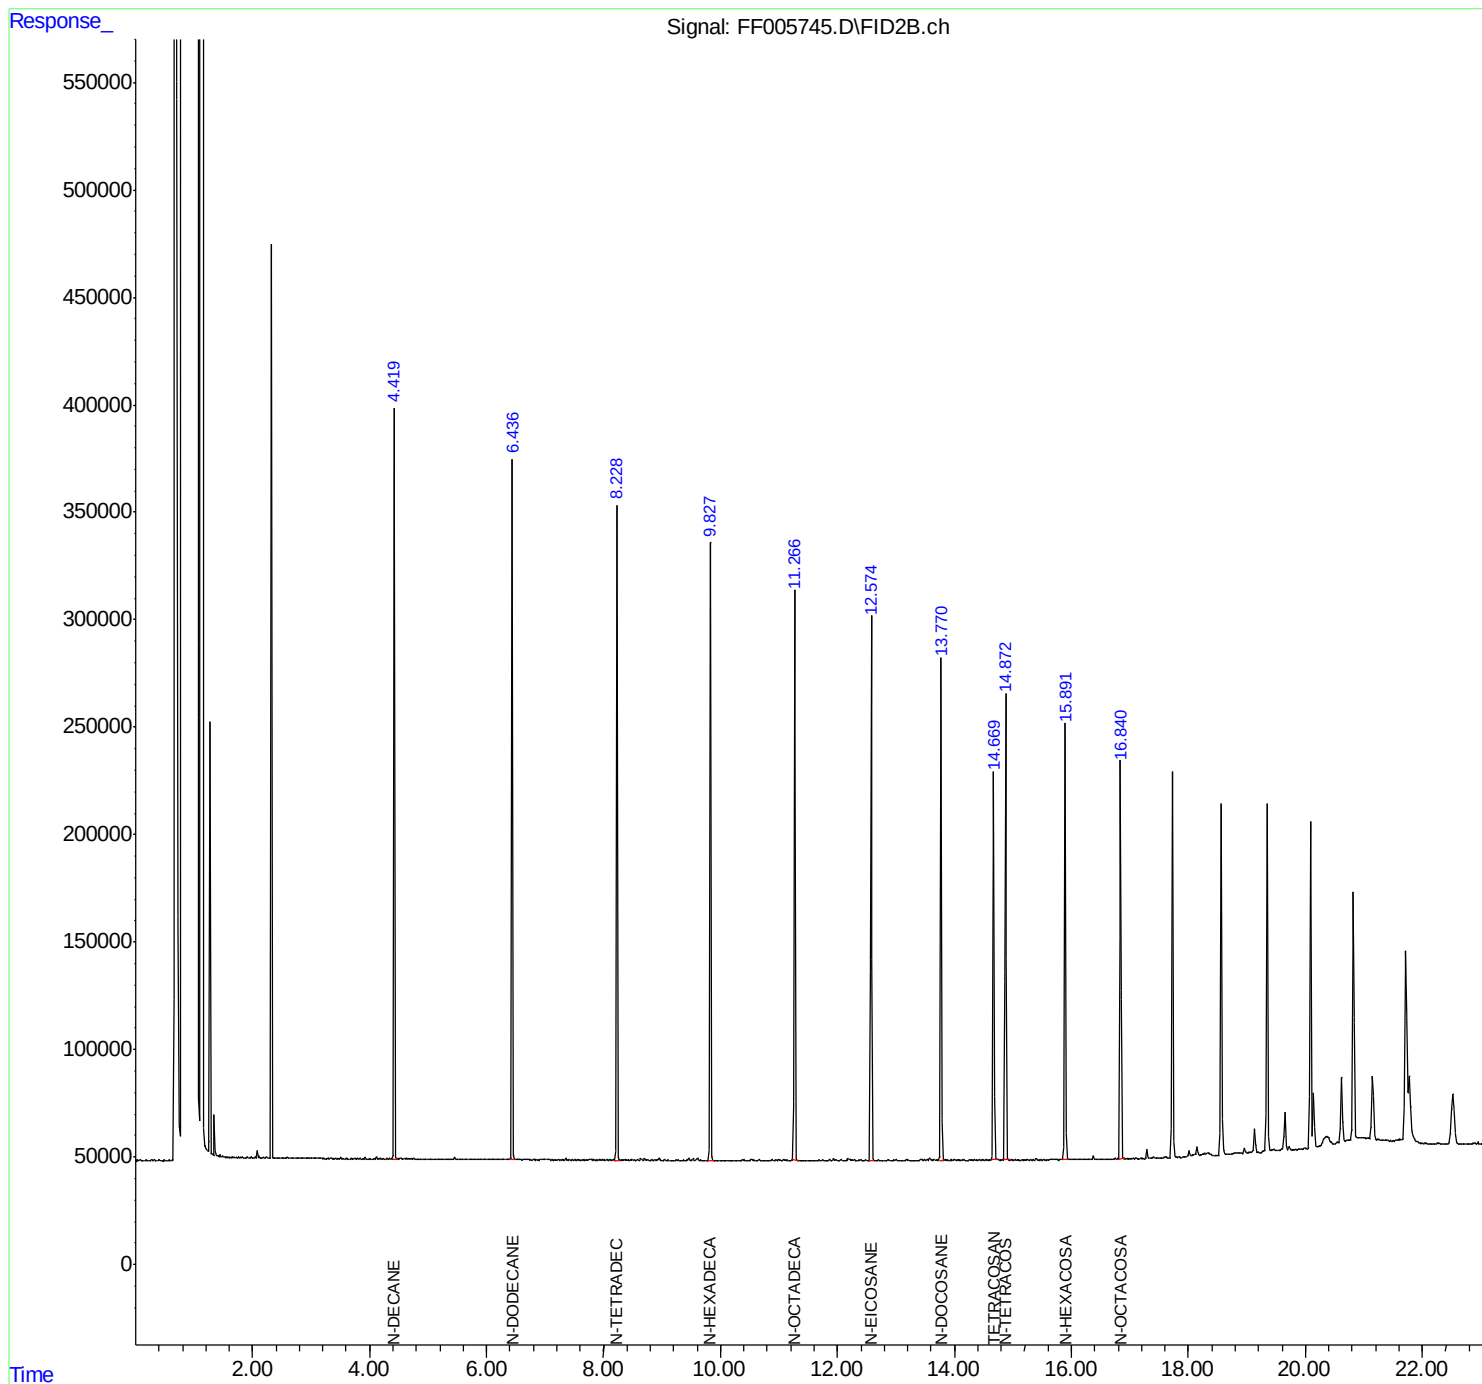

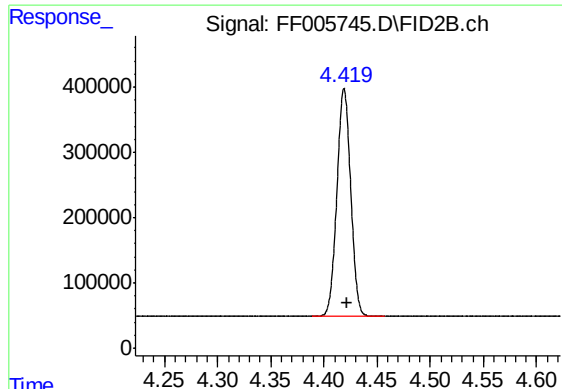


#2 N-DECANE

R.T.: 4.419 min
Delta R.T.: -0.003 min
Response: 3139333
Conc: 20.22 ug/ml

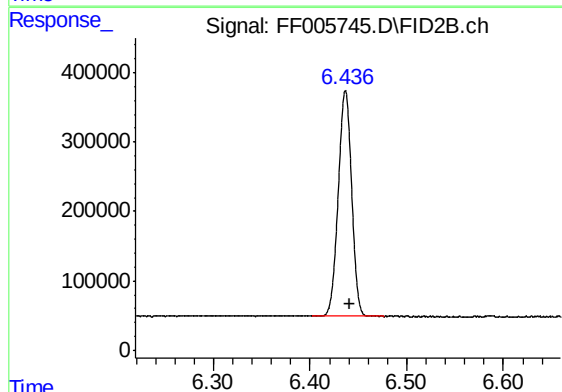


#3 N-DODECANE

R.T.: 6.437 min
Delta R.T.: -0.004 min
Response: 3161749
Conc: 20.08 ug/ml

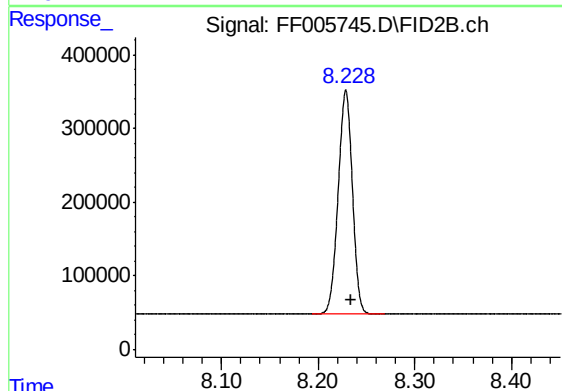


#4 N-TETRADECANE

R.T.: 8.229 min
Delta R.T.: -0.006 min
Response: 3118036
Conc: 19.84 ug/ml

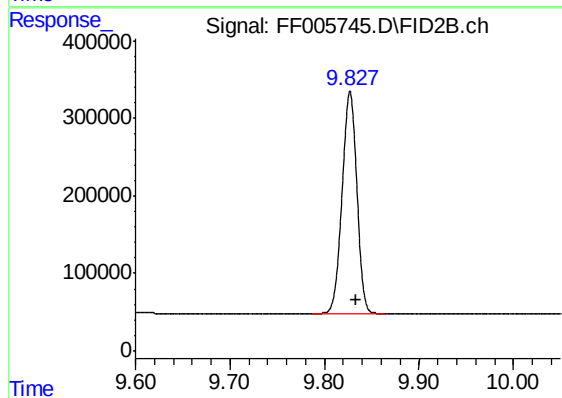


#5 N-HEXADECANE

R.T.: 9.827 min
Delta R.T.: -0.006 min
Response: 3086049
Conc: 19.58 ug/ml

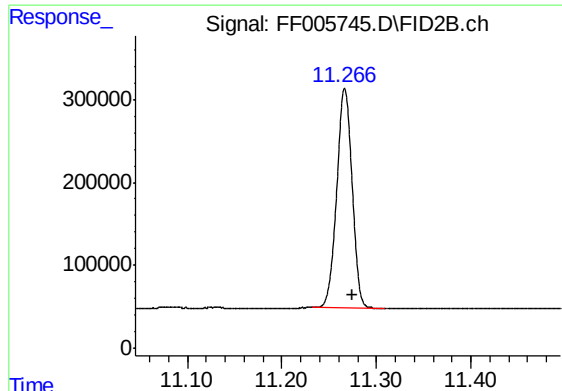


#6 N-OCTADECANE

R.T.: 11.267 min
Delta R.T.: -0.008 min
Response: 2990307
Conc: 19.27 ug/ml

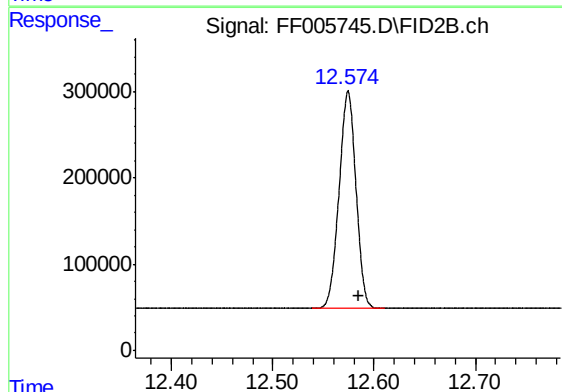


#7 N-EICOSANE

R.T.: 12.574 min
Delta R.T.: -0.010 min
Response: 2932282
Conc: 18.94 ug/ml

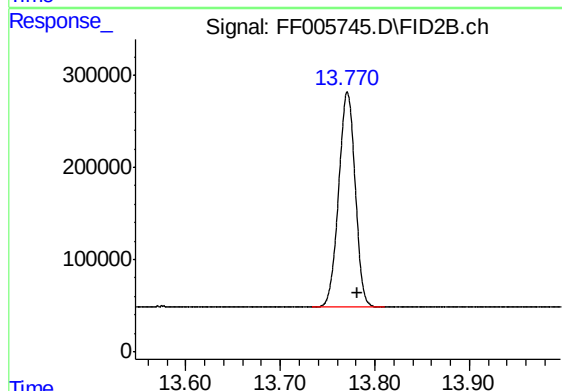


#8 N-DOCOSANE

R.T.: 13.771 min
Delta R.T.: -0.010 min
Response: 2825337
Conc: 18.62 ug/ml

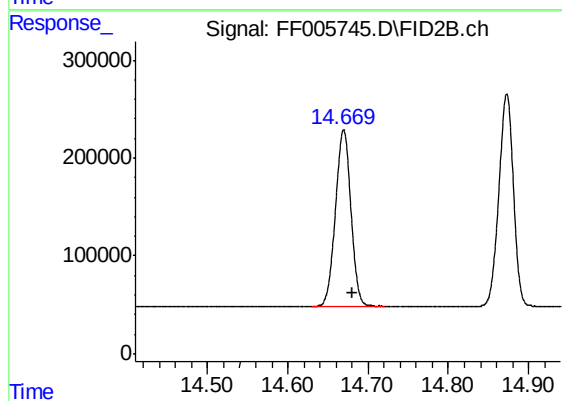


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.670 min
Delta R.T.: -0.011 min
Response: 2401183
Conc: 18.47 ug/ml

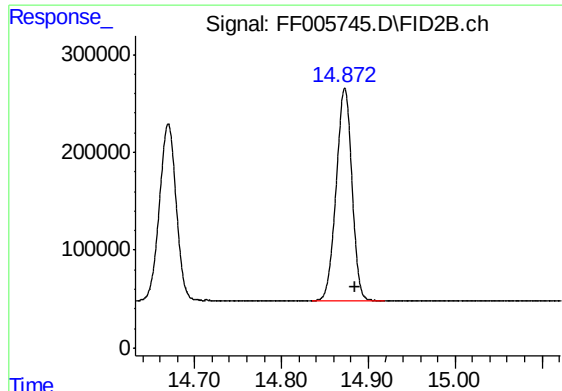


#10 N-TETRACOSANE

R.T.: 14.873 min
Delta R.T.: -0.011 min
Response: 2723863
Conc: 18.31 ug/ml

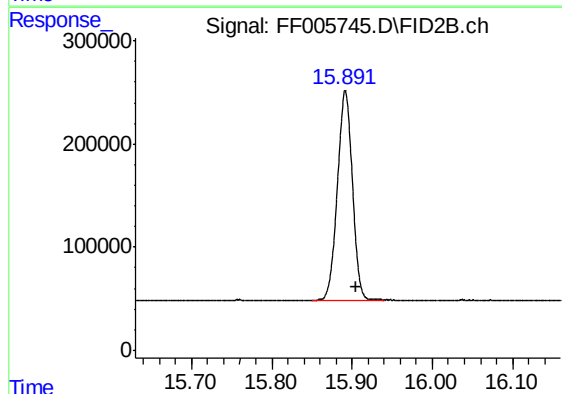

#11 N-HEXACOSANE

R.T.: 15.892 min
Delta R.T.: -0.013 min
Response: 2625915
Conc: 18.00 ug/ml

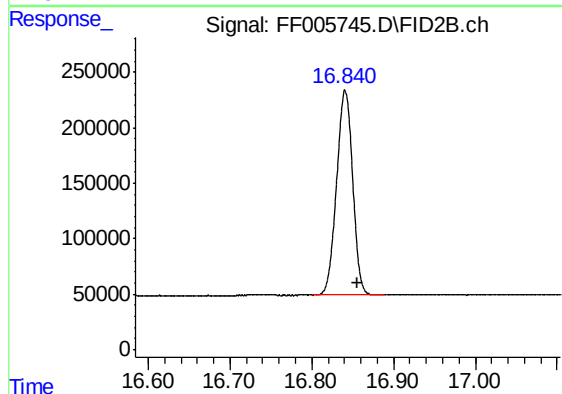

#12 N-OCTACOSANE

R.T.: 16.841 min
Delta R.T.: -0.015 min
Response: 2525824
Conc: 17.74 ug/ml