

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100821\
Data File : FF009081.D
Signal(s) : FID2B.ch
Acq On : 08 Oct 2021 11:21
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 23:54:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.485	2768385	21.791 ug/ml
12)	N-OCTACOSANE	16.878	2766361	23.631 ug/ml
13)	N-TRIACONTANE	17.764	139047	1.232 ug/ml
14)	N-DOTRIACONTANE	18.592	179049	1.696 ug/ml
15)	N-TETRATRIACONTANE	19.373	137780	1.410 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100821\
Data File : FF009081.D
Signal(s) : FID2B.ch
Acq On : 08 Oct 2021 11:21
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 23:54:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

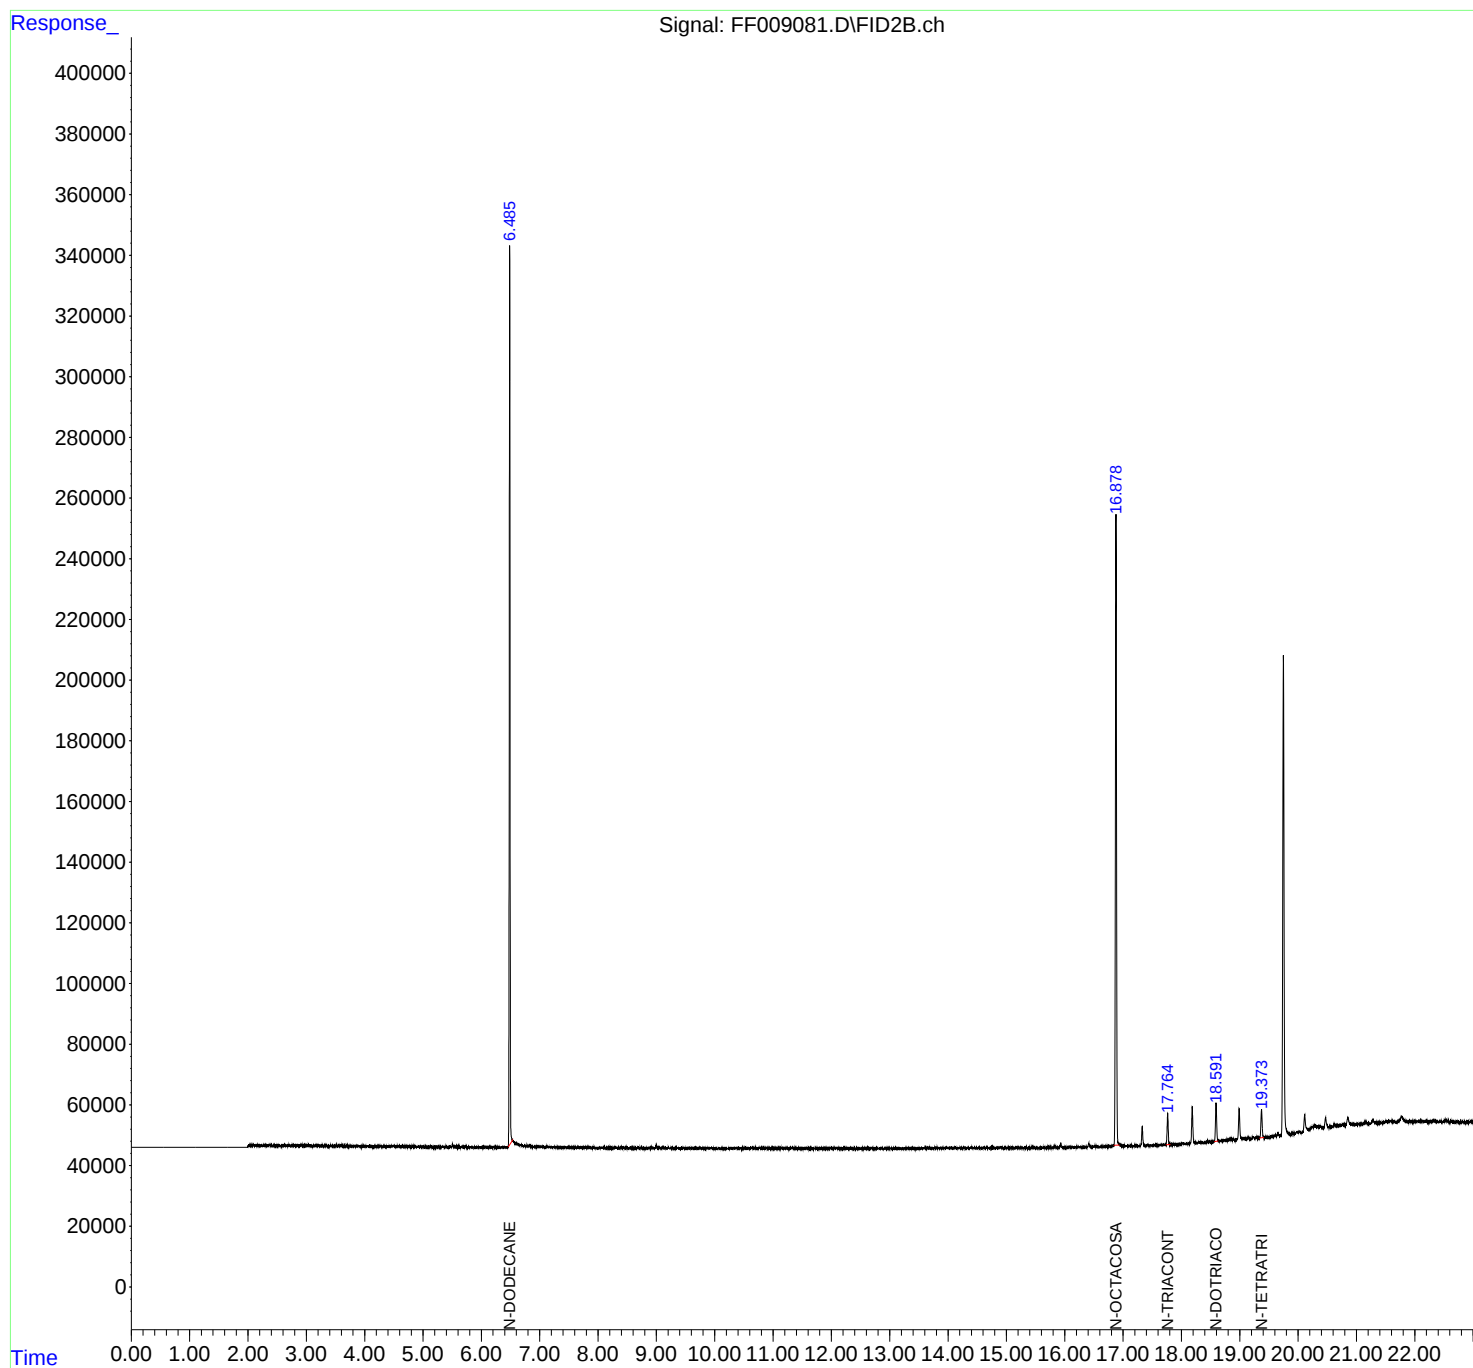


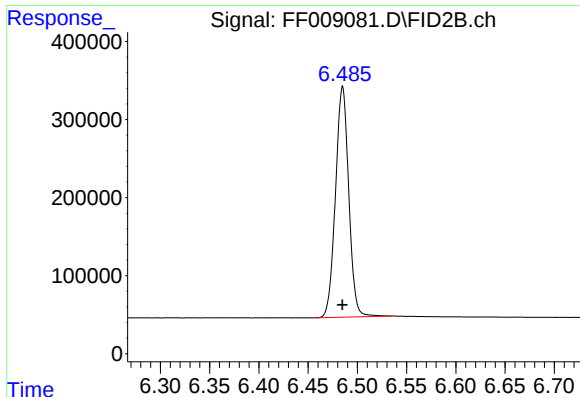

#3 N-DODECANE


R.T.: 6.485 min
Delta R.T.: 0.000 min
Response: 2768385
Conc: 21.79 ug/ml

Instrument :
FID_F
ClientSampleId :

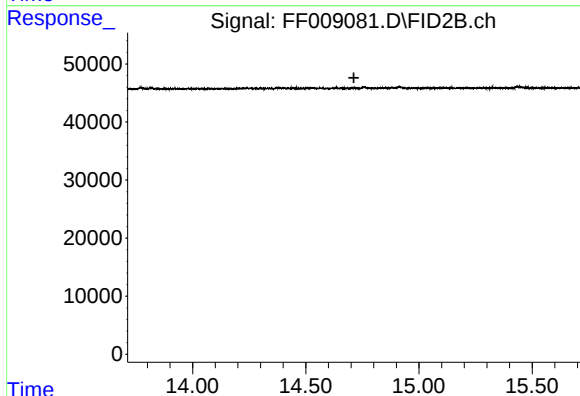


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.

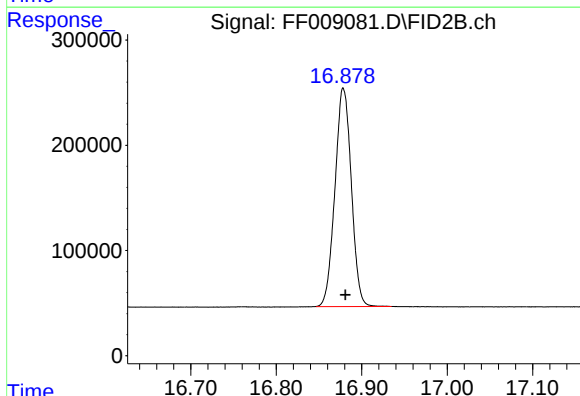


#12 N-OCTACOSANE

R.T.: 16.878 min
Delta R.T.: -0.003 min
Response: 2766361
Conc: 23.63 ug/ml

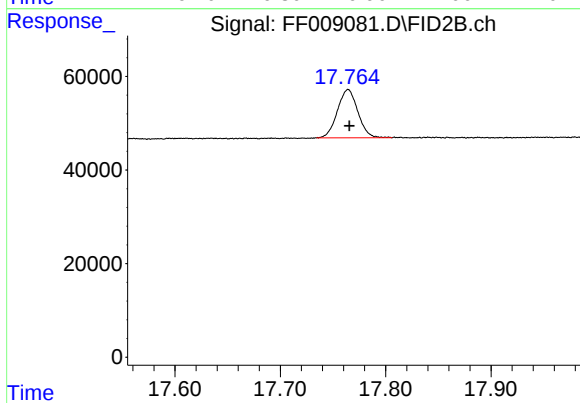

#13 N-TRIACONTANE


R.T.: 17.764 min
Delta R.T.: -0.001 min
Response: 139047
Conc: 1.23 ug/ml

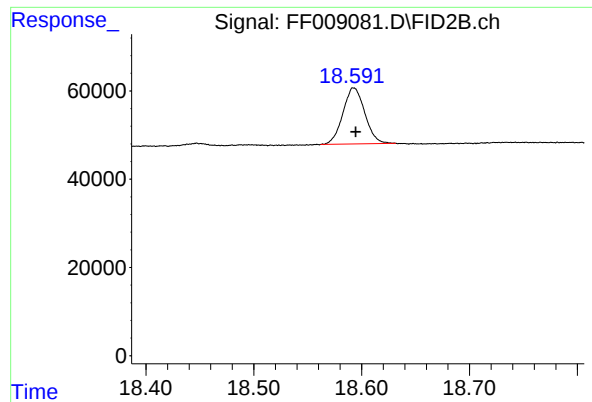

#14 N-DOTRIACONTANE

R.T.: 18.592 min
Delta R.T.: -0.003 min
Response: 179049
Conc: 1.70 ug/ml

Instrument :
FID_F
ClientSampleId :

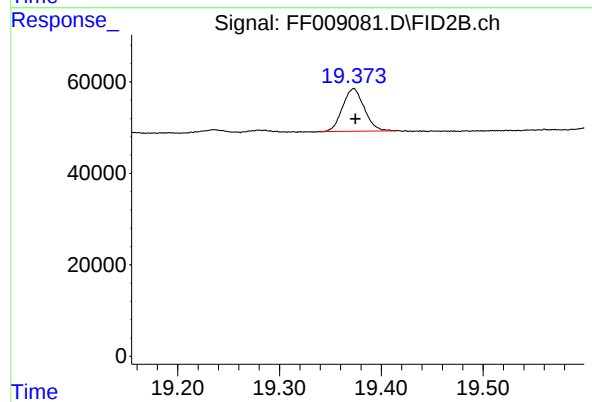

#15 N-TETRATRIACONTANE

R.T.: 19.373 min
Delta R.T.: -0.001 min
Response: 137780
Conc: 1.41 ug/ml