

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100821\
Data File : FF009085.D
Signal(s) : FID2B.ch
Acq On : 08 Oct 2021 13:24
Operator : AJ\MA
Sample : M4089-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
20-SB-2-20211005-5.5-6.0

Integration File: autoint1.e
Quant Time: Oct 08 23:55:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.716	2413329	22.008 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100821\
Data File : FF009085.D
Signal(s) : FID2B.ch
Acq On : 08 Oct 2021 13:24
Operator : AJ\MA
Sample : M4089-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
20-SB-2-20211005-5.5-6.0

Integration File: autoint1.e
Quant Time: Oct 08 23:55:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

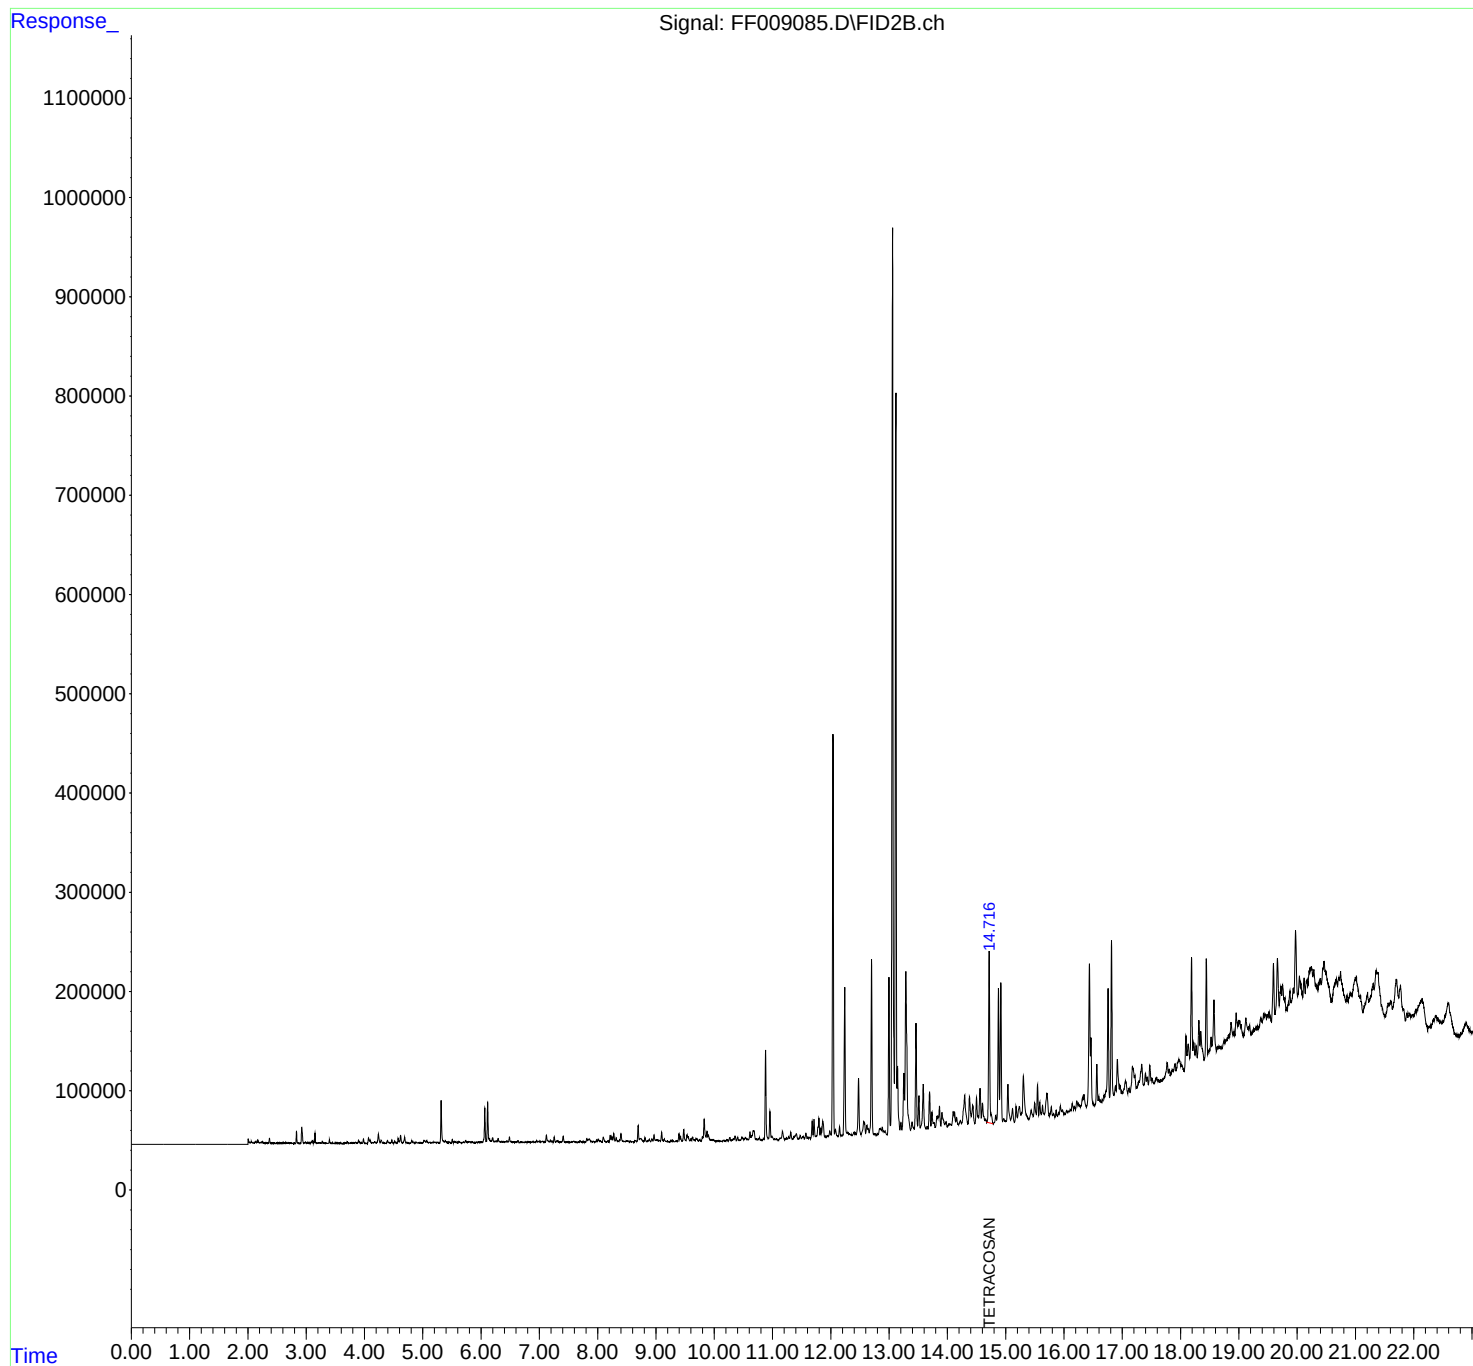

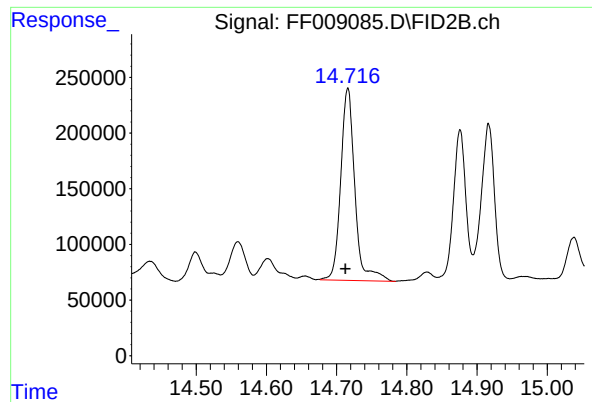

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.716 min
Delta R.T.: 0.004 min
Response: 2413329
Conc: 22.01 ug/ml

Instrument :
FID_F
ClientSampleId :
20-SB-2-20211005-5.5-6.0