

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100821\
Data File : FF009088.D
Signal(s) : FID2B.ch
Acq On : 08 Oct 2021 14:56
Operator : AJ\MA
Sample : M4089-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
20-SB-2-20211005-5.5-6.0-A

Integration File: autoint1.e
Quant Time: Oct 08 23:56:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	2234373	20.376 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100821\
Data File : FF009088.D
Signal(s) : FID2B.ch
Acq On : 08 Oct 2021 14:56
Operator : AJ\MA
Sample : M4089-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
20-SB-2-20211005-5.5-6.0-A

Integration File: autoint1.e
Quant Time: Oct 08 23:56:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

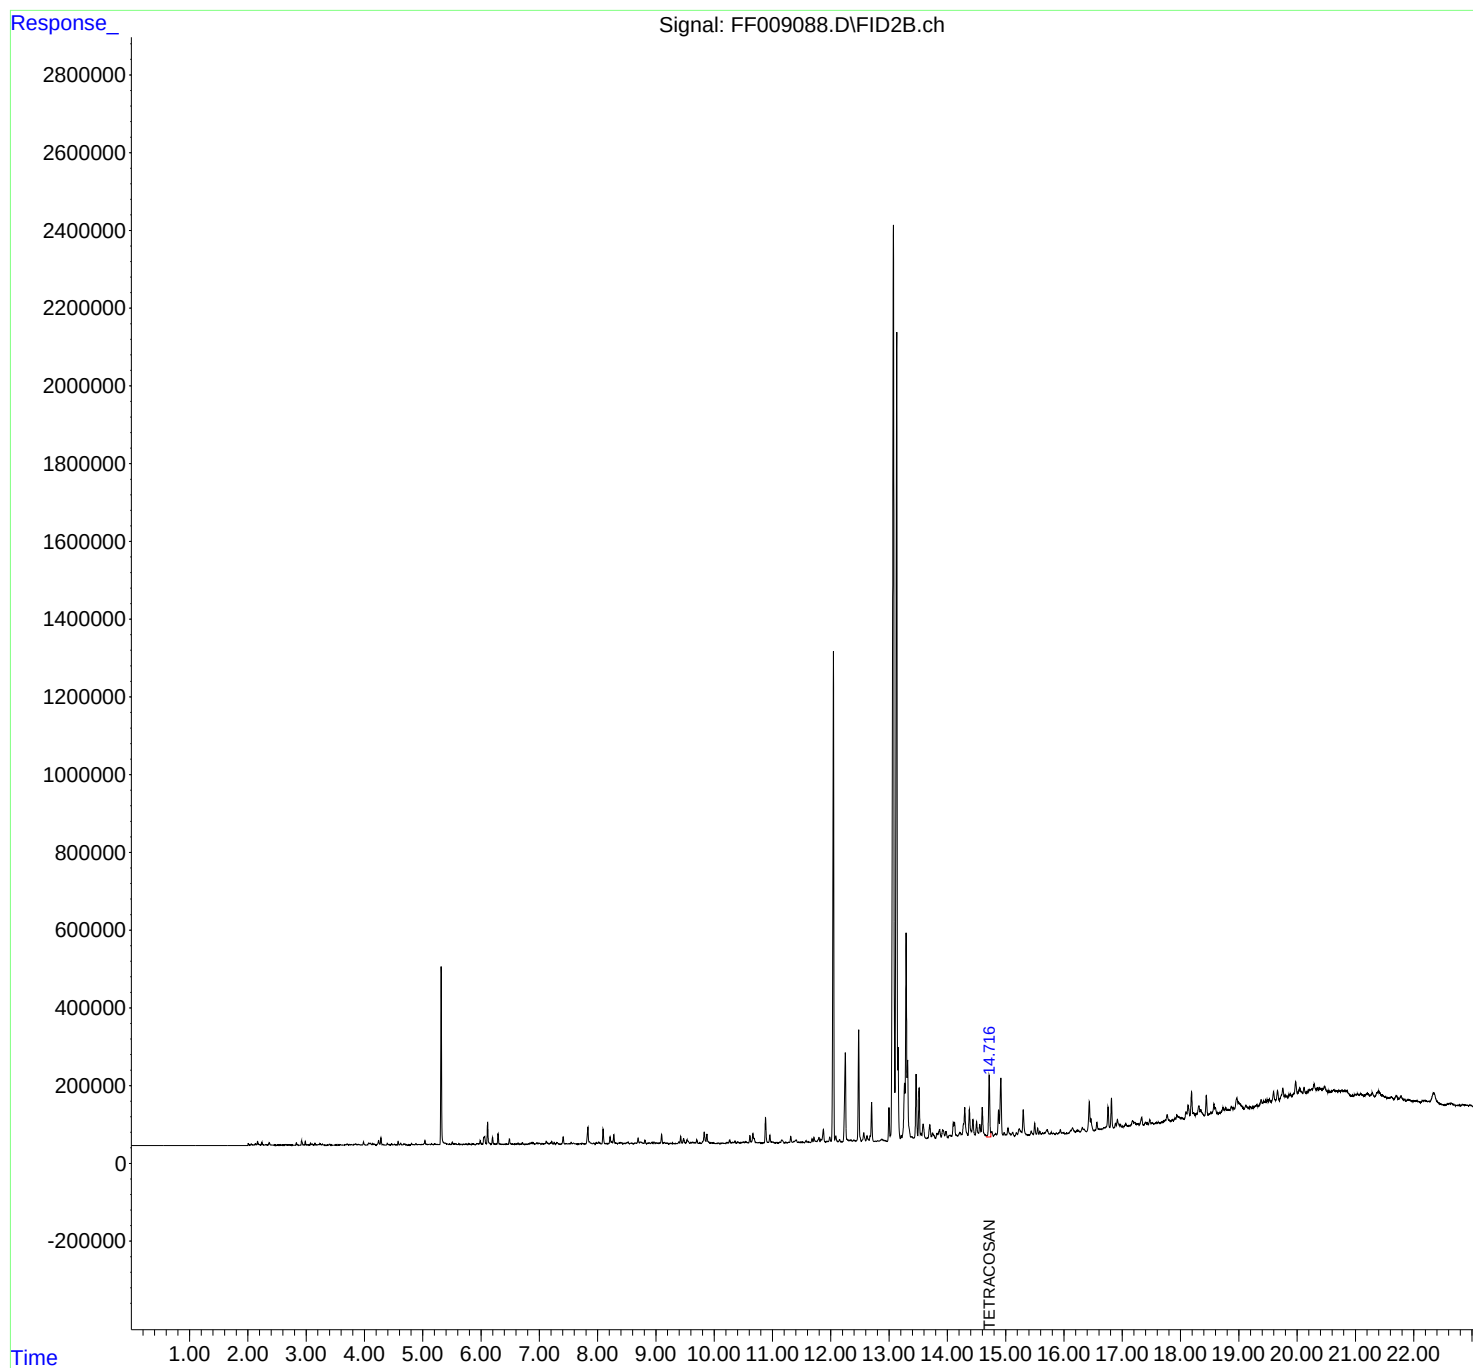

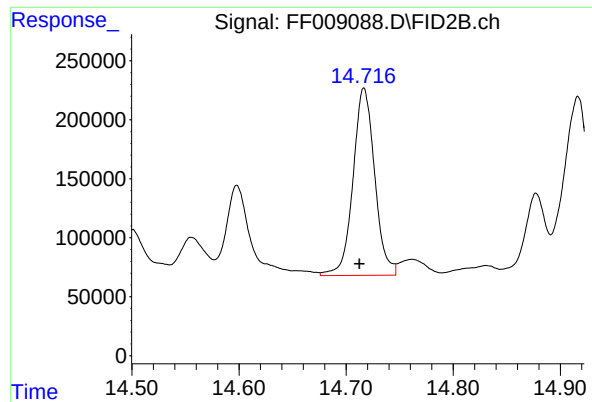

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.717 min
Delta R.T.: 0.004 min
Response: 2234373
Conc: 20.38 ug/ml

Instrument :
FID_F
ClientSampleId :
20-SB-2-20211005-5.5-6.0-A