

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100821\
Data File : FF009091.D
Signal(s) : FID2B.ch
Acq On : 08 Oct 2021 16:29
Operator : AJ\MA
Sample : M4057-01 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SHAFT-17B-SP

Integration File: autoint1.e
Quant Time: Oct 08 23:57:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.719	164929	1.504 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100821\
Data File : FF009091.D
Signal(s) : FID2B.ch
Acq On : 08 Oct 2021 16:29
Operator : AJ\MA
Sample : M4057-01 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SHAFT-17B-SP

Integration File: autoint1.e
Quant Time: Oct 08 23:57:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

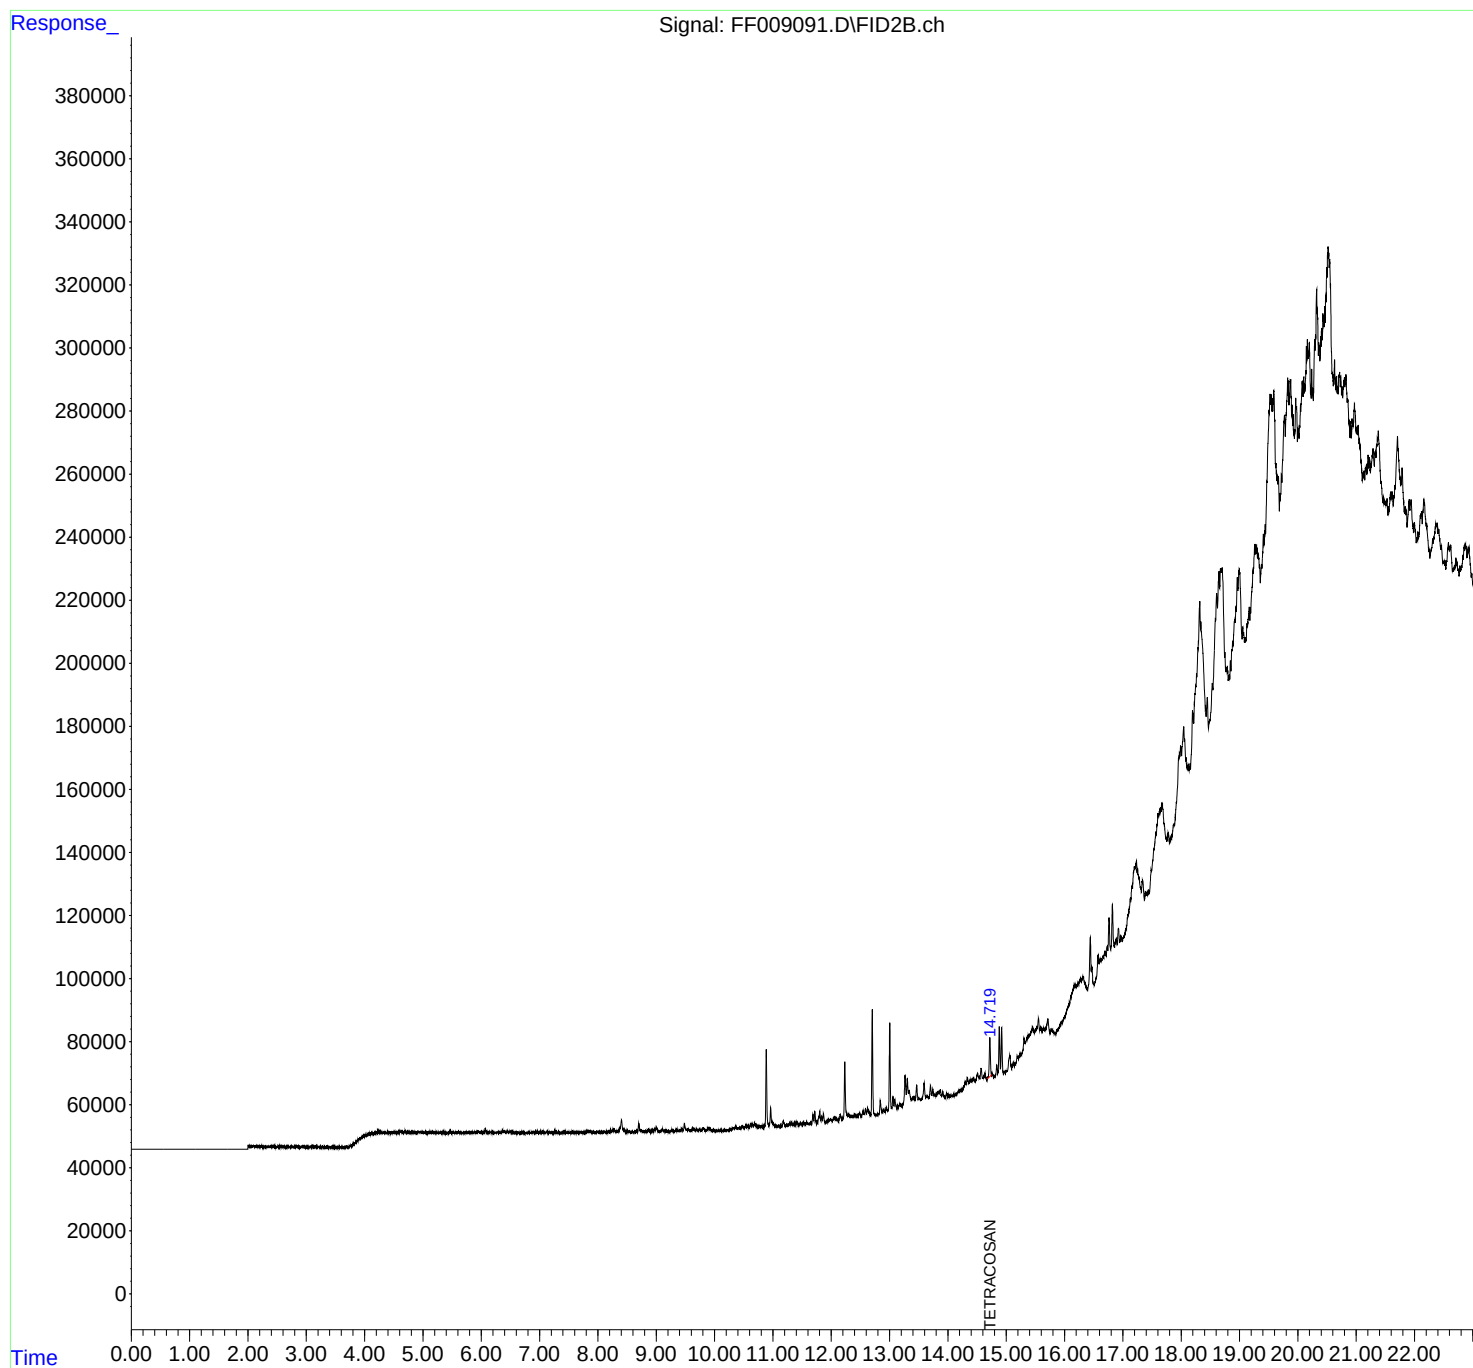

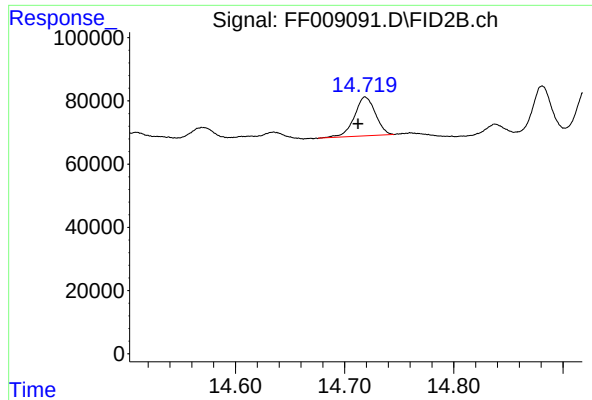

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.719 min
Delta R.T.: 0.006 min
Response: 164929
Conc: 1.50 ug/ml

Instrument :
FID_F
ClientSampleId :
SHAFT-17B-SP