

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100918\
 Data File : FF002378.D
 Signal(s) : FID2B.ch
 Acq On : 09 Oct 2018 12:51
 Operator : AJ\SJ
 Sample : PB113653BS
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 09 16:27:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.654	1785031	12.516 ug/ml
Target Compounds			
2) N-DECANE	4.374	2314577	14.289 ug/ml
3) N-DODECANE	6.399	2399983	14.589 ug/ml
4) N-TETRADECANE	8.194	2408676	14.460 ug/ml
5) N-HEXADECANE	9.797	2417300	14.434 ug/ml
6) N-OCTADECANE	11.240	2404384	14.320 ug/ml
7) N-EICOSANE	12.553	2341801	14.140 ug/ml
8) N-DOCOSANE	13.753	2269382	13.908 ug/ml
10) N-TETRACOSANE	14.858	2183856	13.658 ug/ml
11) N-HEXACOSANE	15.882	2092501	13.360 ug/ml
12) N-OCTACOSANE	16.832	2022446	13.221 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100918\
Data File : FF002378.D
Signal(s) : FID2B.ch
Acq On : 09 Oct 2018 12:51
Operator : AJ\SJ
Sample : PB113653BS
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 09 16:27:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

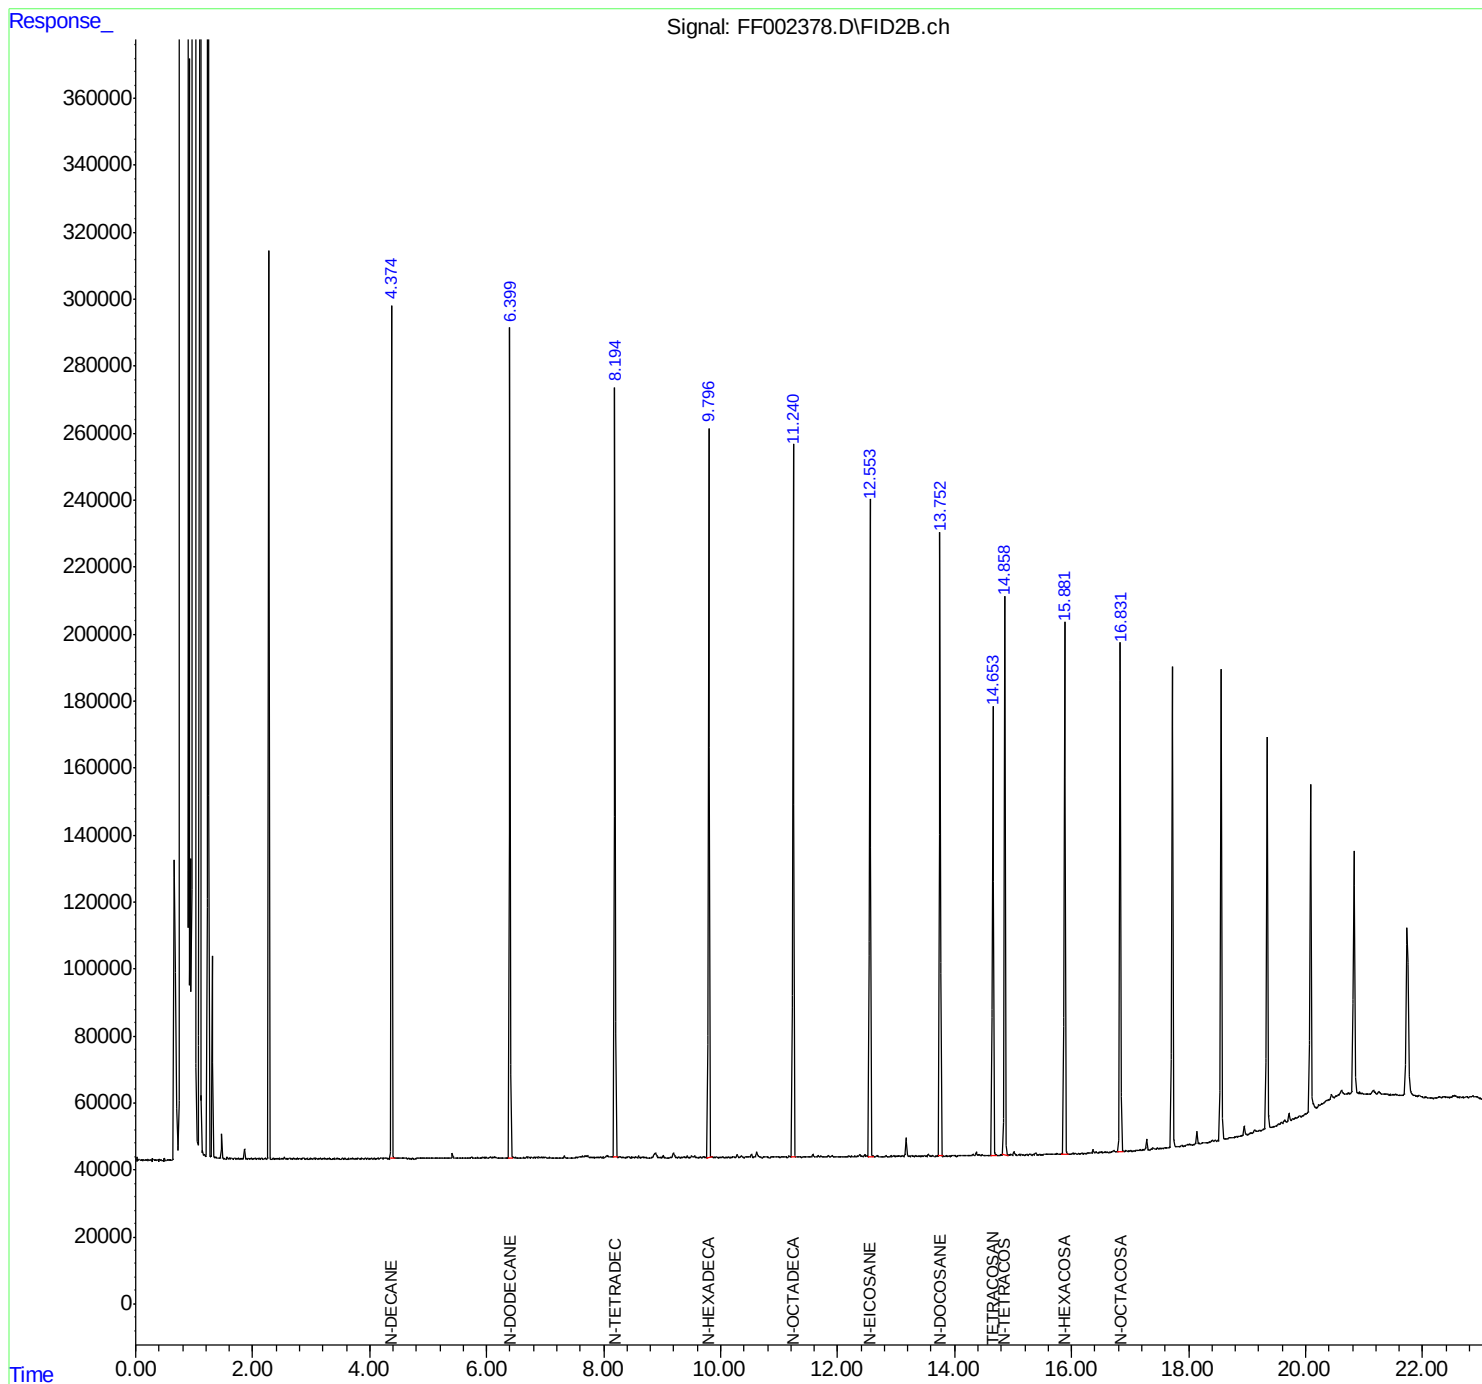

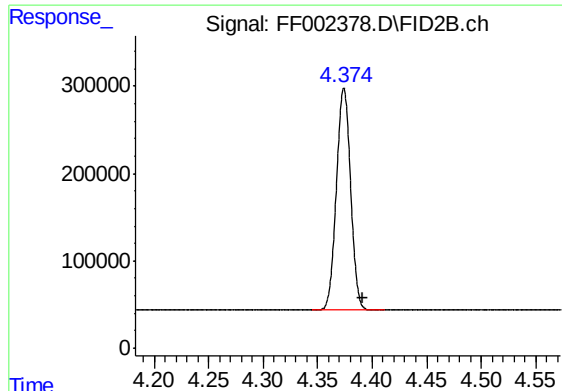


#2 N-DECANE

R.T.: 4.374 min
Delta R.T.: -0.017 min
Response: 2314577
Conc: 14.29 ug/ml

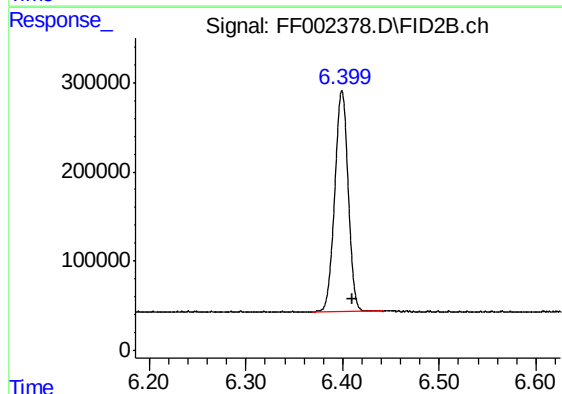


#3 N-DODECANE

R.T.: 6.399 min
Delta R.T.: -0.011 min
Response: 2399983
Conc: 14.59 ug/ml

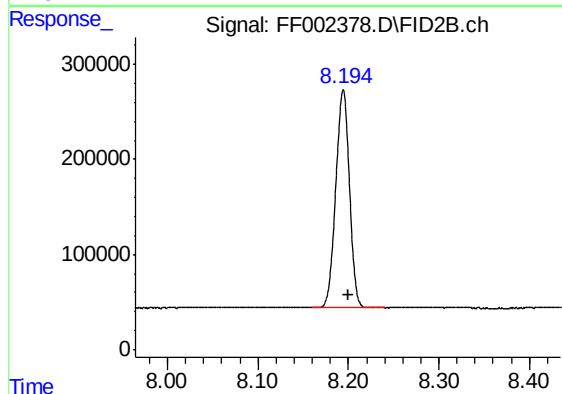


#4 N-TETRADECANE

R.T.: 8.194 min
Delta R.T.: -0.006 min
Response: 2408676
Conc: 14.46 ug/ml

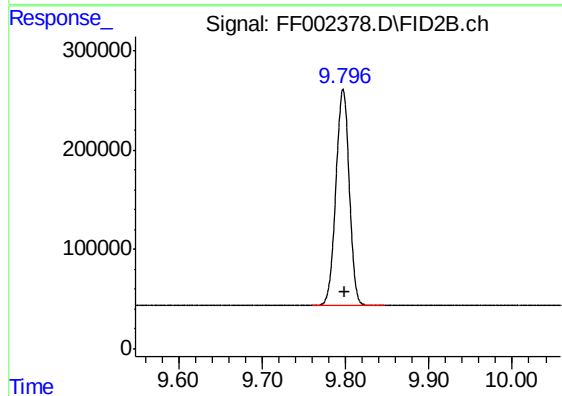


#5 N-HEXADECANE

R.T.: 9.797 min
Delta R.T.: -0.001 min
Response: 2417300
Conc: 14.43 ug/ml

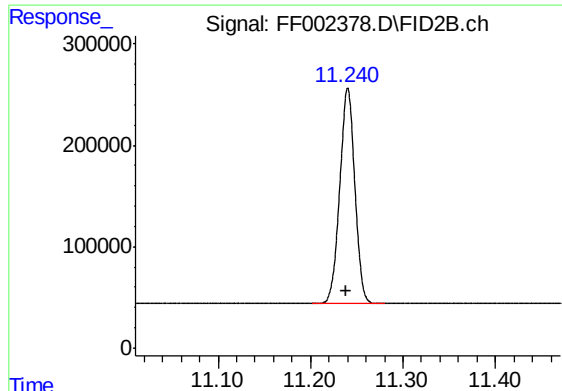


#6 N-OCTADECANE

R.T.: 11.240 min
Delta R.T.: 0.002 min
Response: 2404384
Conc: 14.32 ug/ml

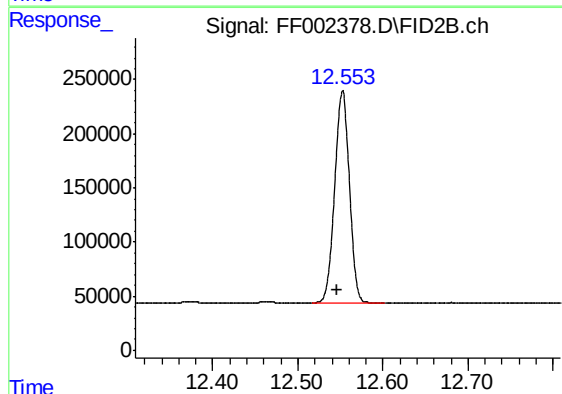


#7 N-EICOSANE

R.T.: 12.553 min
Delta R.T.: 0.006 min
Response: 2341801
Conc: 14.14 ug/ml

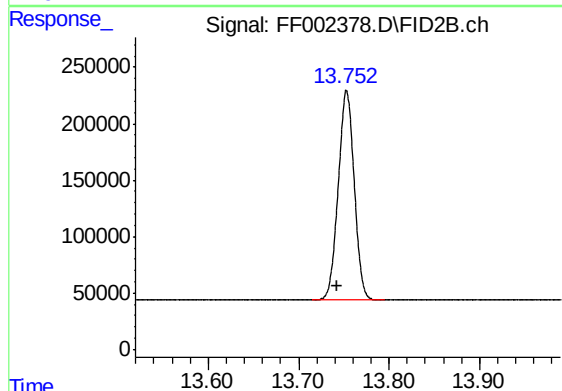


#8 N-DOCOSANE

R.T.: 13.753 min
Delta R.T.: 0.010 min
Response: 2269382
Conc: 13.91 ug/ml

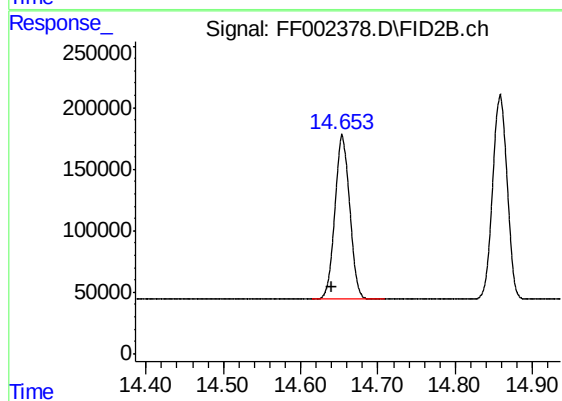


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.654 min
Delta R.T.: 0.013 min
Response: 1785031
Conc: 12.52 ug/ml

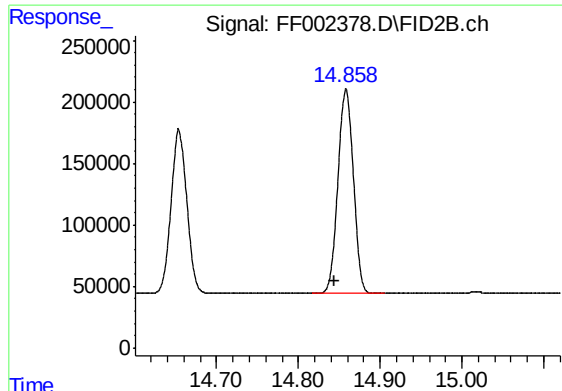


#10 N-TETRACOSANE

R.T.: 14.858 min
Delta R.T.: 0.014 min
Response: 2183856
Conc: 13.66 ug/ml

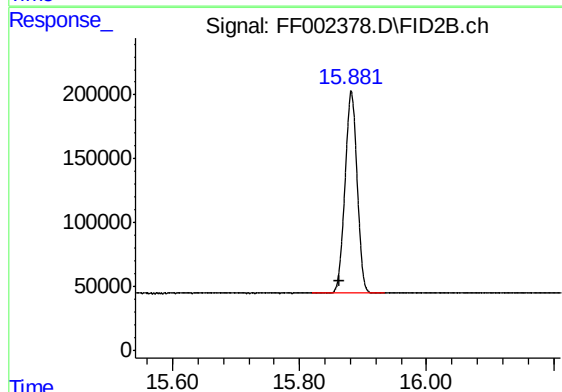

#11 N-HEXACOSANE

R.T.: 15.882 min
Delta R.T.: 0.018 min
Response: 2092501
Conc: 13.36 ug/ml

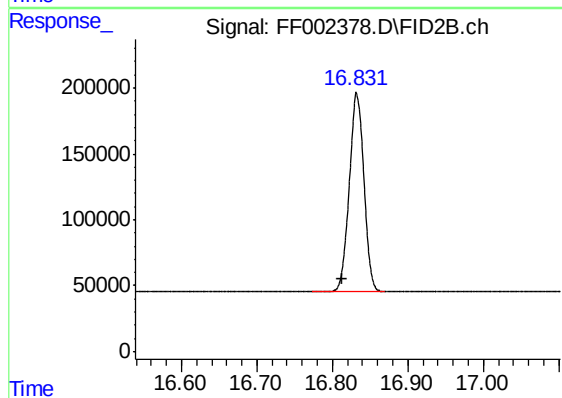

#12 N-OCTACOSANE

R.T.: 16.832 min
Delta R.T.: 0.020 min
Response: 2022446
Conc: 13.22 ug/ml