

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100923AL\
 Data File : FF013575.D
 Signal(s) : FID2B.ch
 Acq On : 09 Oct 2023 08:53
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 09 23:48:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100623.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 07 07:01:38 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.351	299792	2.501 ug/ml
Spiked Amount 50.000		Recovery =	5.00%
Target Compounds			
10) T n-Eicosane (C20)	12.866	330583	2.428 ug/ml
14) T n-Tetracosane (C24)	15.165	295597	2.164 ug/ml
16) T n-Octacosane (C28)	17.092f	172332	1.289 ug/ml
17) T n-Tricontane (C30)	18.079	243780	1.760 ug/ml
18) T n-Dotriacontane (C32)	18.887	807000	5.874 ug/ml
19) T n-Tetratriacontane (C34)	19.584f	254367	1.964 ug/ml
20) T n-Hexatriacontane (C36)	20.381	230084	1.845 ug/ml
21) T n-Octatriacontane (C38)	21.176f	244580	2.081 ug/ml
22) T n-Tetracontane (C40)	22.060f	1009793	8.779 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100923AL\
Data File : FF013575.D
Signal(s) : FID2B.ch
Acq On : 09 Oct 2023 08:53
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 09 23:48:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100623.M
Quant Title : GC Extractables
QLast Update : Sat Oct 07 07:01:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

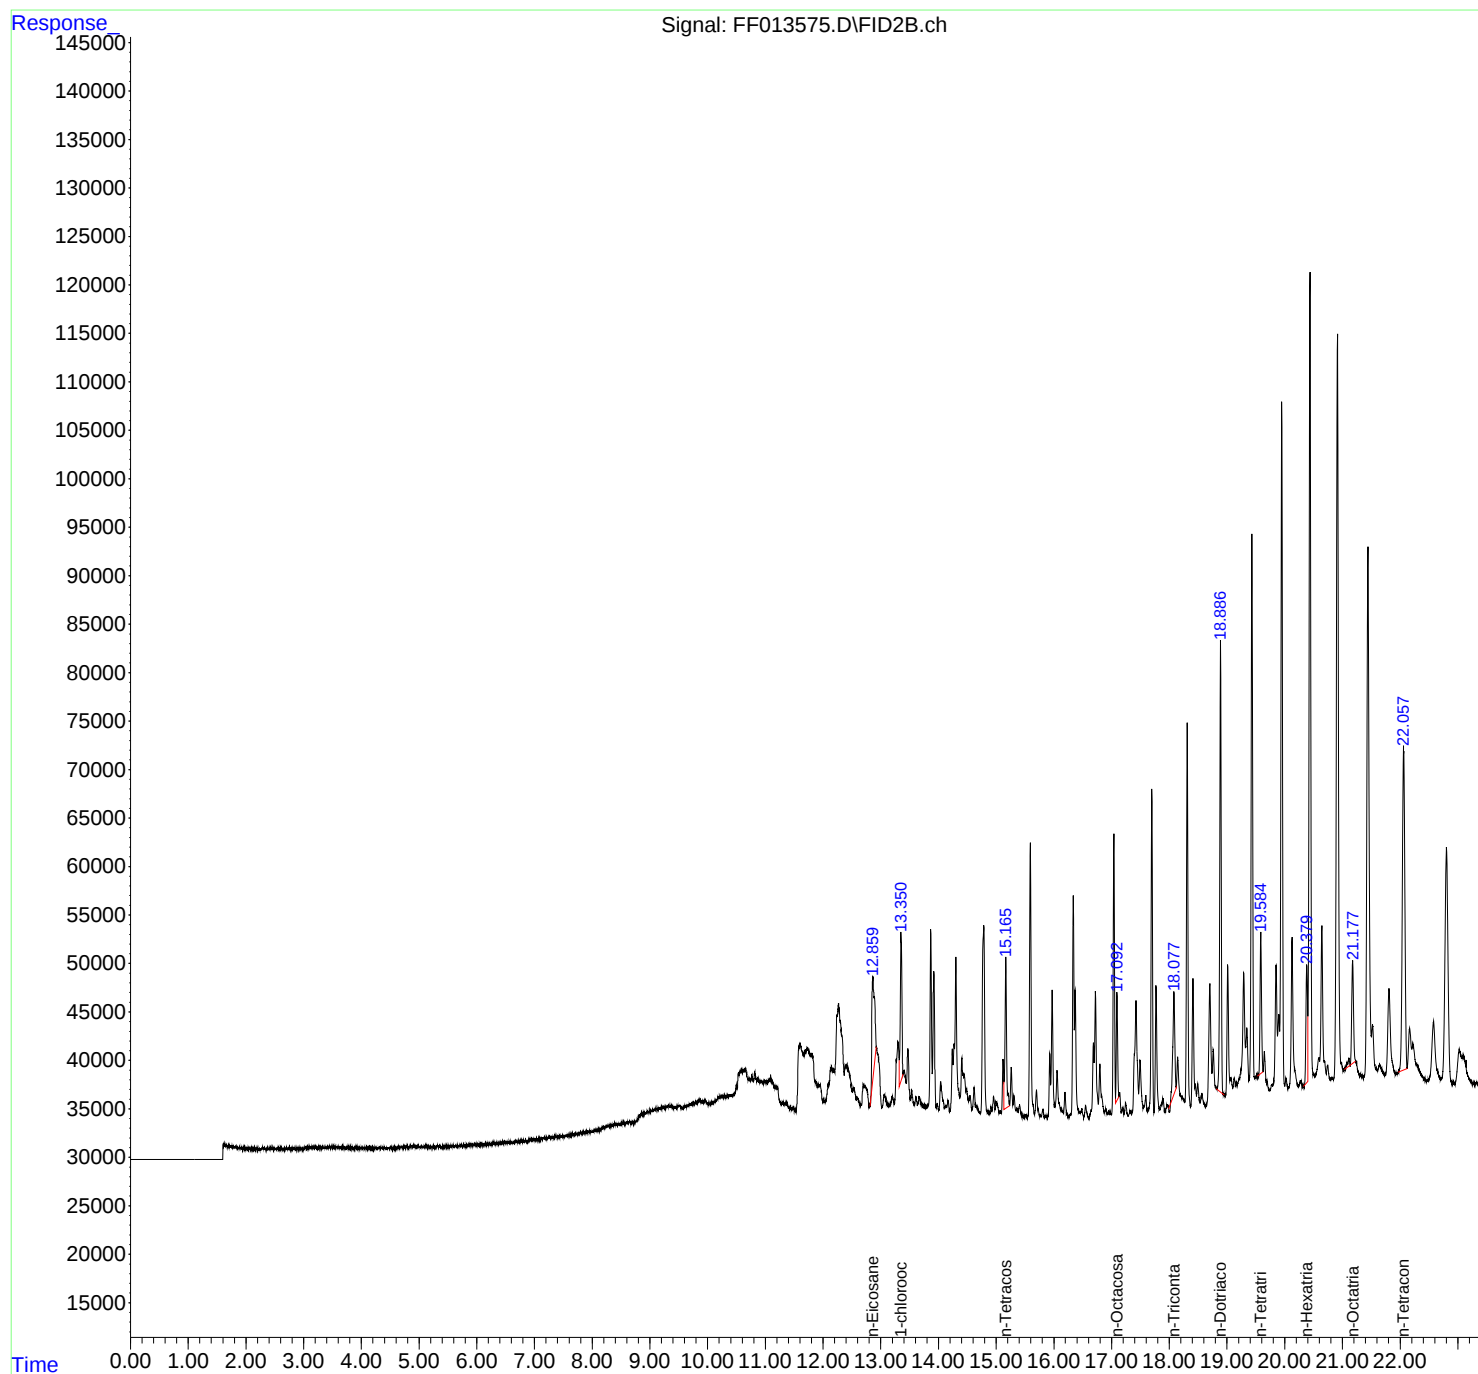


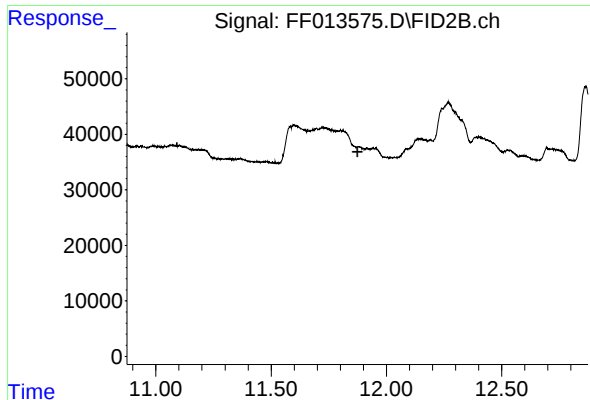

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.875 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

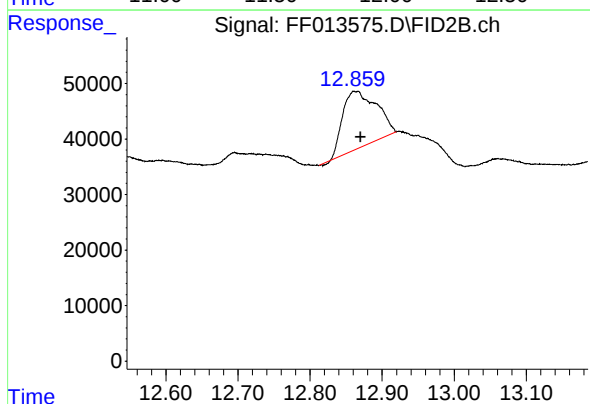


#10 n-Eicosane (C20)

R.T.: 12.866 min
Delta R.T.: -0.004 min
Response: 330583
Conc: 2.43 ug/ml

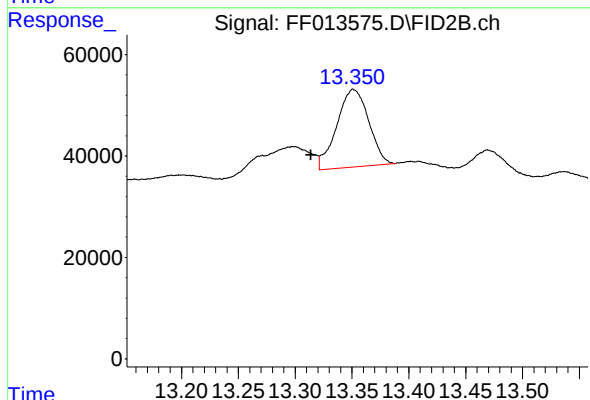


#12 1-chlorooctadecane (SURR)

R.T.: 13.351 min
Delta R.T.: 0.037 min
Response: 299792
Conc: 2.50 ug/ml

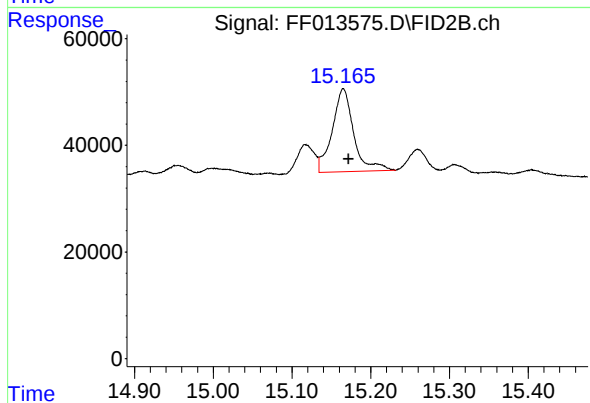

#14 n-Tetracosane (C24)


R.T.: 15.165 min
Delta R.T.: -0.007 min
Response: 295597
Conc: 2.16 ug/ml

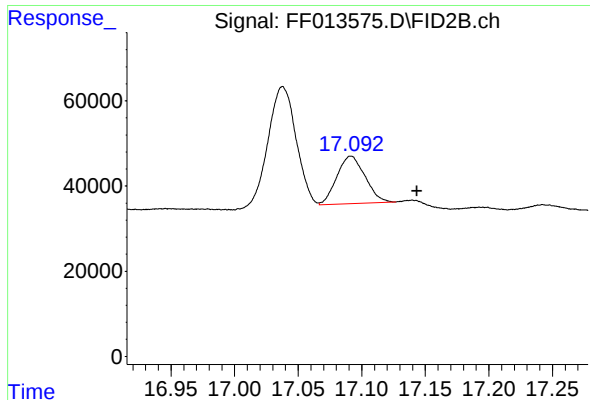

#16 n-Octacosane (C28)


R.T.: 17.092 min
Delta R.T.: -0.052 min
Response: 172332
Conc: 1.29 ug/ml

Instrument :
FID_F
ClientSampleId :

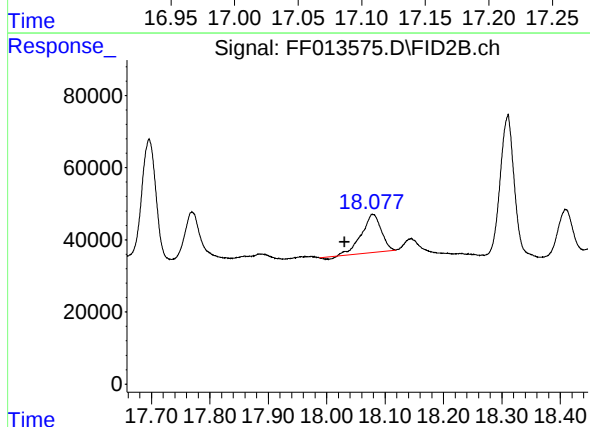


#17 n-Tricontane (C30)

R.T.: 18.079 min
Delta R.T.: 0.048 min
Response: 243780
Conc: 1.76 ug/ml

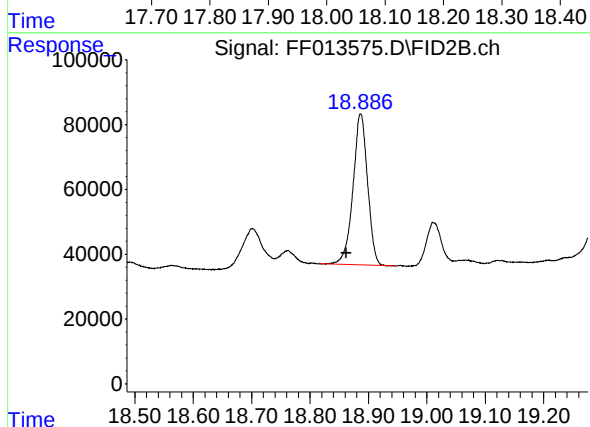


#18 n-Dotriacontane (C32)

R.T.: 18.887 min
Delta R.T.: 0.024 min
Response: 807000
Conc: 5.87 ug/ml

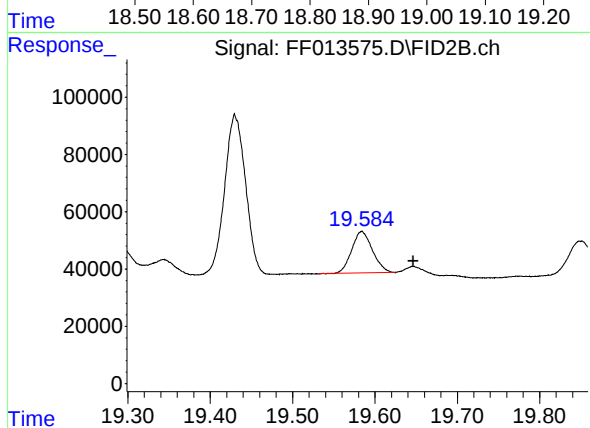

#19 n-Tetratriacontane (C34)


R.T.: 19.584 min
Delta R.T.: -0.063 min
Response: 254367
Conc: 1.96 ug/ml

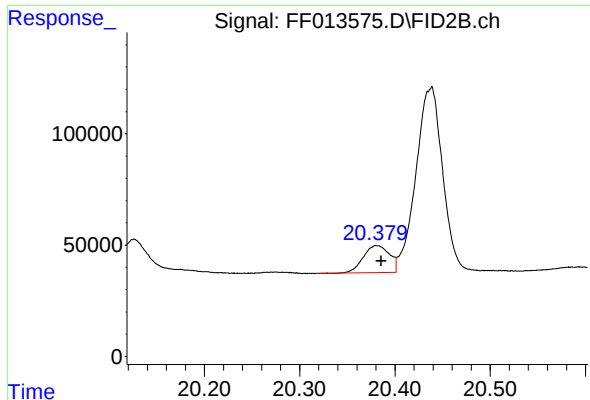

#20 n-Hexatriacontane (C36)


R.T.: 20.381 min
Delta R.T.: -0.005 min
Response: 230084
Conc: 1.84 ug/ml

Instrument :
FID_F
ClientSampleId :

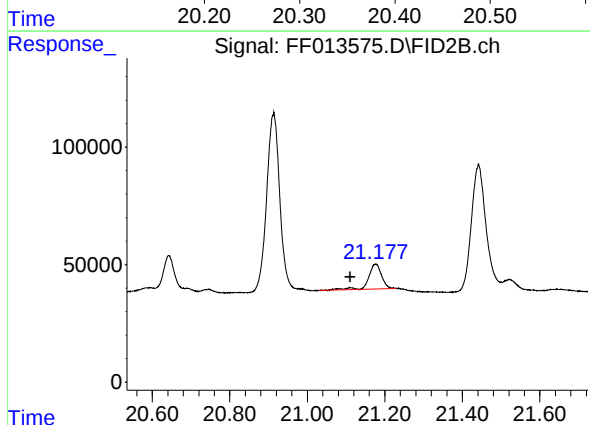

#21 n-Octatriacontane (C38)

R.T.: 21.176 min
Delta R.T.: 0.065 min
Response: 244580
Conc: 2.08 ug/ml

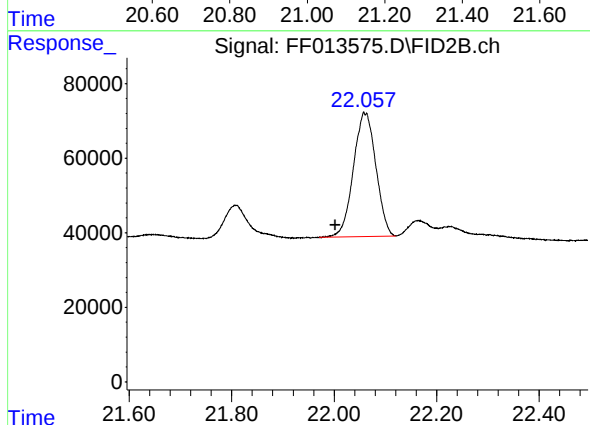

#22 n-Tetracontane (C40)

R.T.: 22.060 min
Delta R.T.: 0.058 min
Response: 1009793
Conc: 8.78 ug/ml