

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF100923AL\  
 Data File : FF013579.D  
 Signal(s) : FID2B.ch  
 Acq On : 09 Oct 2023 10:53  
 Operator : YP\AJ  
 Sample : PB156102BL  
 Misc :  
 ALS Vial : 64 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Oct 09 23:48:51 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\Aliphatic EPH 100623.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Oct 07 07:01:38 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 13.314 | 4383887    | 36.580 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 73.16%       |
|                                |        |            |              |
| Target Compounds               |        |            |              |
| 6) T n-Tetradecane (C14)       | 8.510  | 146354     | 1.149 ug/ml  |
| 7) T n-Hexadecane (C16)        | 10.117 | 172925     | 1.309 ug/ml  |
| 8) T n-Octadecane (C18)        | 11.559 | 105382     | 0.770 ug/ml  |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF100923AL\  
Data File : FF013579.D  
Signal(s) : FID2B.ch  
Acq On : 09 Oct 2023 10:53  
Operator : YP\AJ  
Sample : PB156102BL  
Misc :  
ALS Vial : 64 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Oct 09 23:48:51 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\Aliphatic EPH 100623.M  
Quant Title : GC Extractables  
QLast Update : Sat Oct 07 07:01:38 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

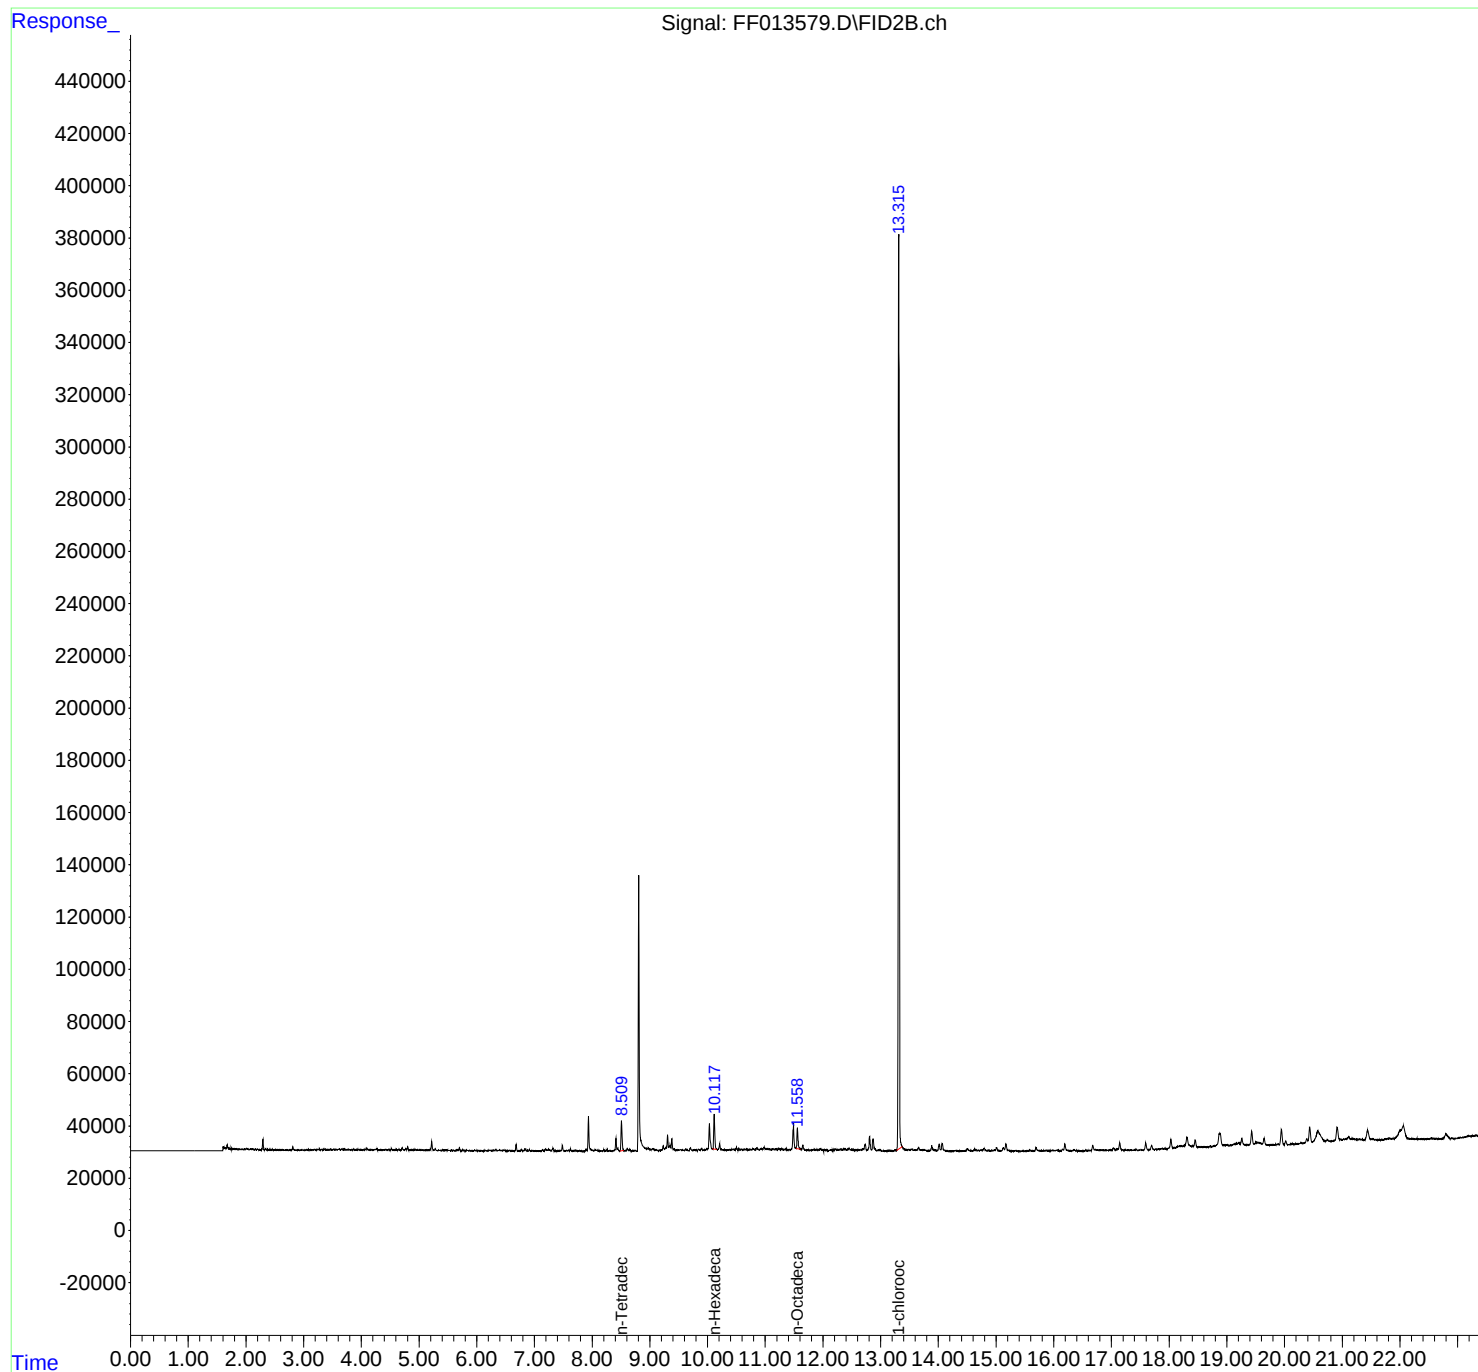


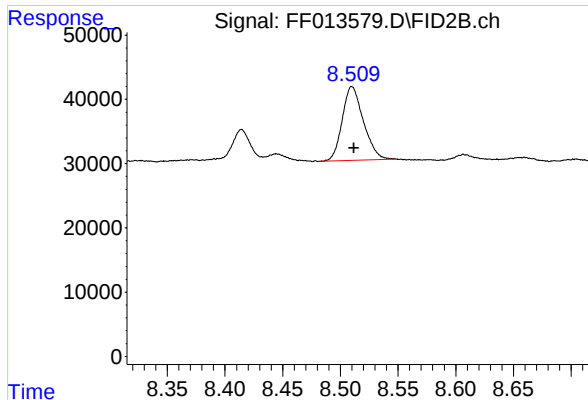

#6 n-Tetradecane (C14)


R.T.: 8.510 min  
Delta R.T.: -0.002 min  
Response: 146354  
Conc: 1.15 ug/ml

Instrument : FID\_F  
ClientSampleId :

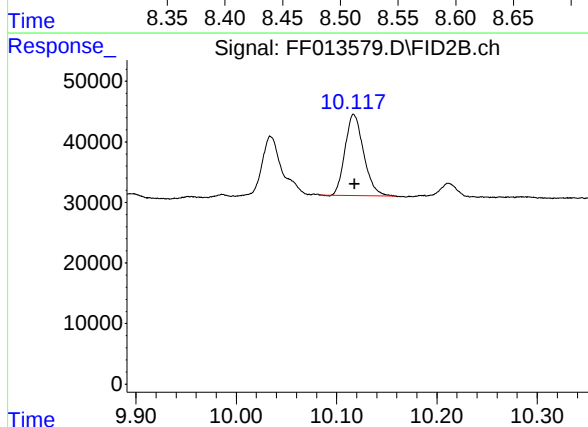


#7 n-Hexadecane (C16)

R.T.: 10.117 min  
Delta R.T.: 0.000 min  
Response: 172925  
Conc: 1.31 ug/ml

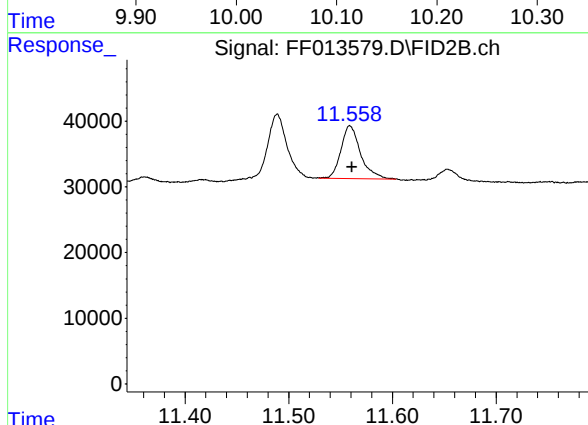


#8 n-Octadecane (C18)

R.T.: 11.559 min  
Delta R.T.: -0.002 min  
Response: 105382  
Conc: 0.77 ug/ml

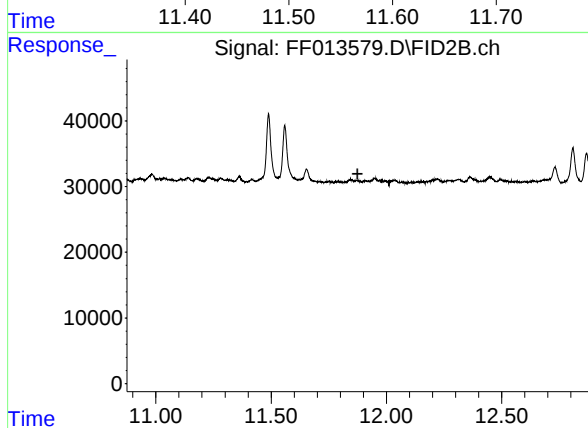

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.875 min  
Response: 0  
Conc: N.D.

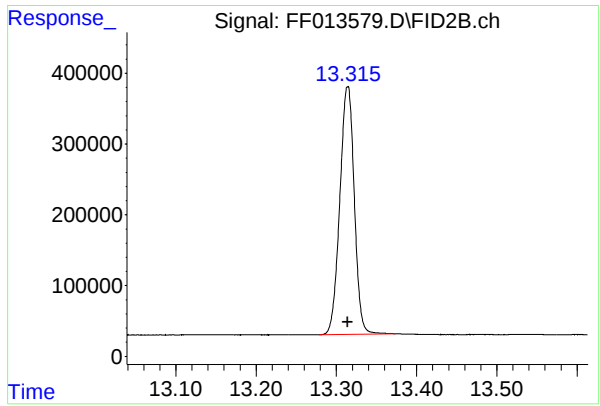

#12 1-chlorooctadecane (SURR)

R.T.: 13.314 min  
Delta R.T.: 0.000 min  
Response: 4383887  
Conc: 36.58 ug/ml

Instrument :  
FID\_F  
ClientSampleId :