

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101018\
 Data File : FF002393.D
 Signal(s) : FID2B.ch
 Acq On : 10 Oct 2018 15:05
 Operator : AJ\SJ
 Sample : J5200-07 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 11 02:00:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.656	344023	2.412 ug/ml
Target Compounds			
4) N-TETRADECANE	8.258f	145406	0.873 ug/ml
7) N-EICOSANE	12.494f	106462	0.643 ug/ml
8) N-DOCOSANE	13.774	101304	0.621 ug/ml
10) N-TETRACOSANE	14.825	203615	1.273 ug/ml
12) N-OCTACOSANE	16.830	83717	0.547 ug/ml
13) N-TRIACONTANE	17.723	208452	1.394 ug/ml
14) N-DOTRIACONTANE	18.557	146520	1.017 ug/ml
15) N-TETRATRIACONTANE	19.344	66410	0.478 ug/ml
16) N-HEXATRIACONTANE	20.087	71941	0.558 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101018\
Data File : FF002393.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2018 15:05
Operator : AJ\SJ
Sample : J5200-07 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 11 02:00:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

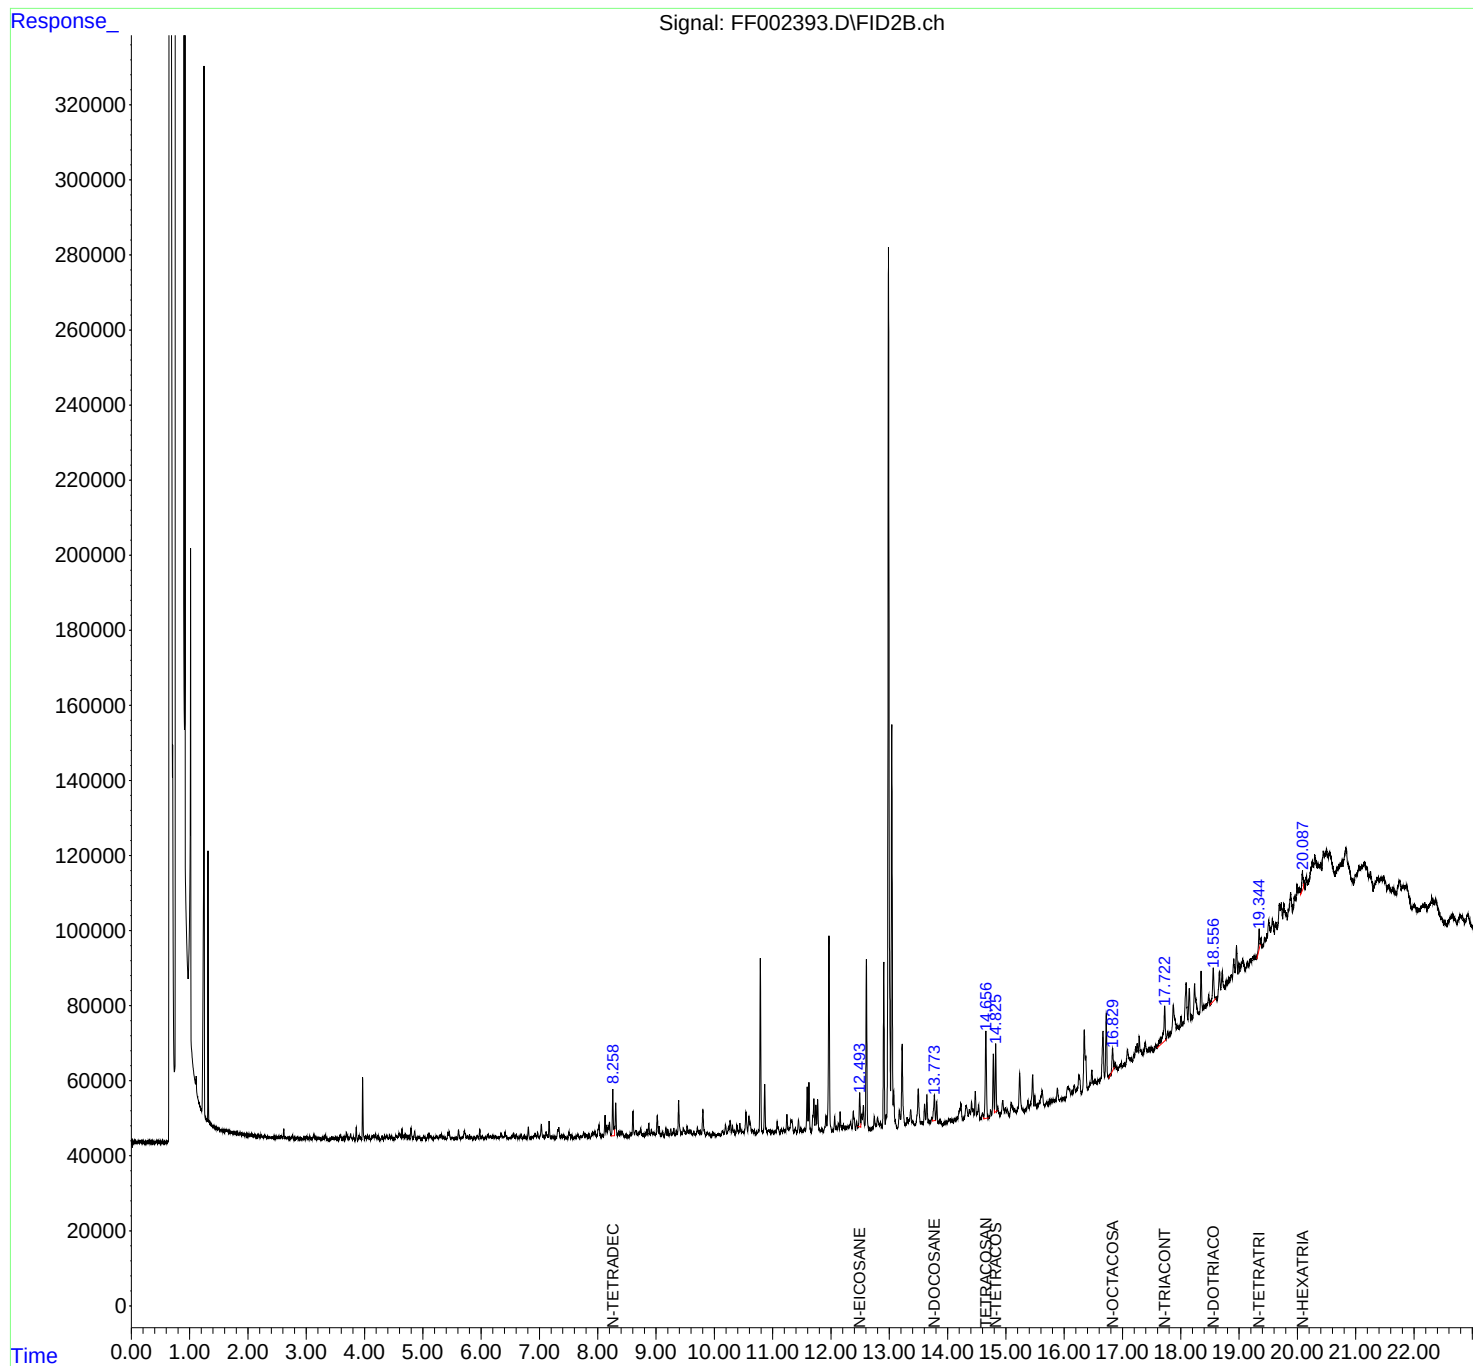

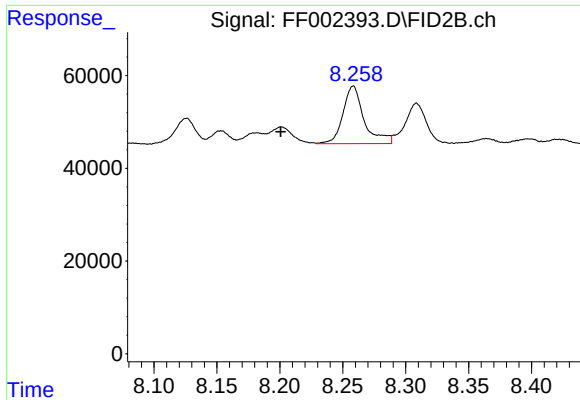


#4 N-TETRADECANE

R.T.: 8.258 min
Delta R.T.: 0.058 min
Response: 145406
Conc: 0.87 ug/ml

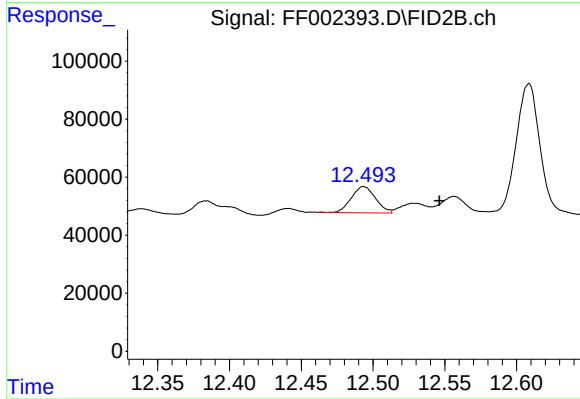


#7 N-EICOSANE

R.T.: 12.494 min
Delta R.T.: -0.053 min
Response: 106462
Conc: 0.64 ug/ml

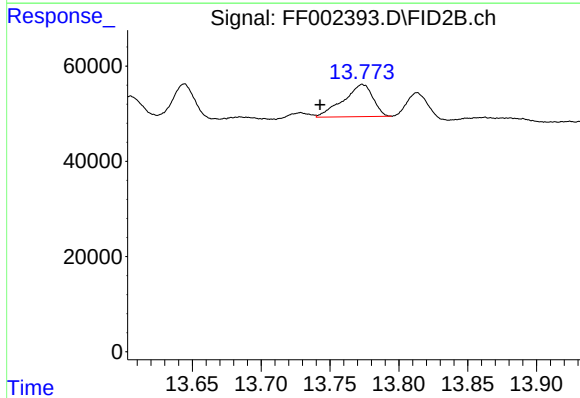


#8 N-DOCOSANE

R.T.: 13.774 min
Delta R.T.: 0.031 min
Response: 101304
Conc: 0.62 ug/ml

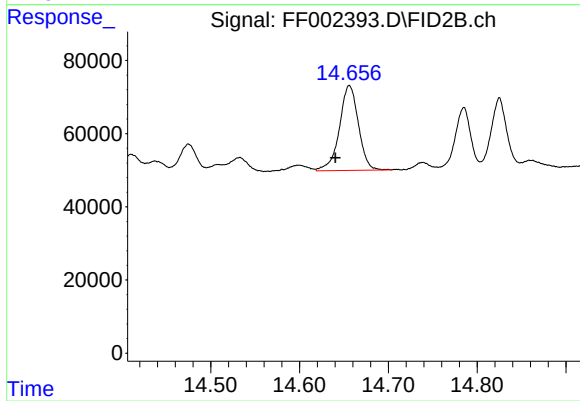


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.656 min
Delta R.T.: 0.016 min
Response: 344023
Conc: 2.41 ug/ml

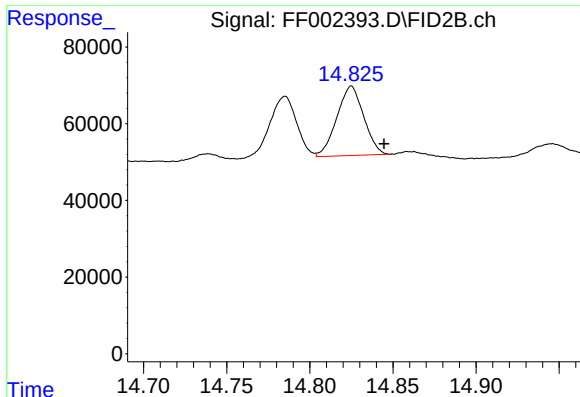


#10 N-TETRACOSANE

R.T.: 14.825 min
Delta R.T.: -0.020 min
Response: 203615
Conc: 1.27 ug/ml

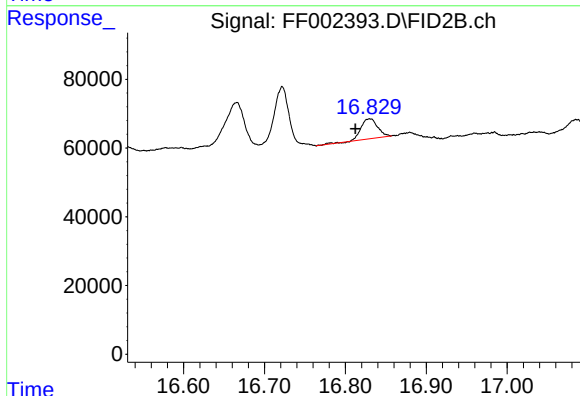


#12 N-OCTACOSANE

R.T.: 16.830 min
Delta R.T.: 0.018 min
Response: 83717
Conc: 0.55 ug/ml

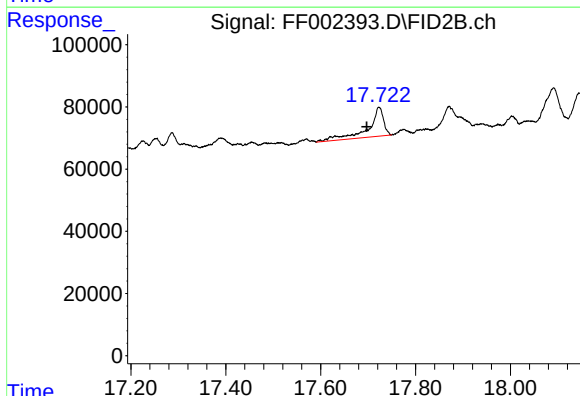


#13 N-TRIACONTANE

R.T.: 17.723 min
Delta R.T.: 0.026 min
Response: 208452
Conc: 1.39 ug/ml

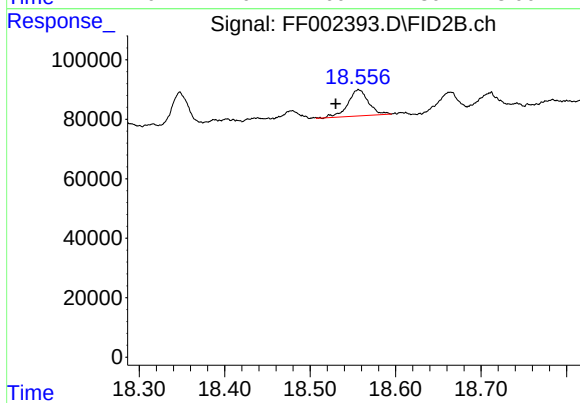

#14 N-DOTRIACONTANE

R.T.: 18.557 min
Delta R.T.: 0.027 min
Response: 146520
Conc: 1.02 ug/ml

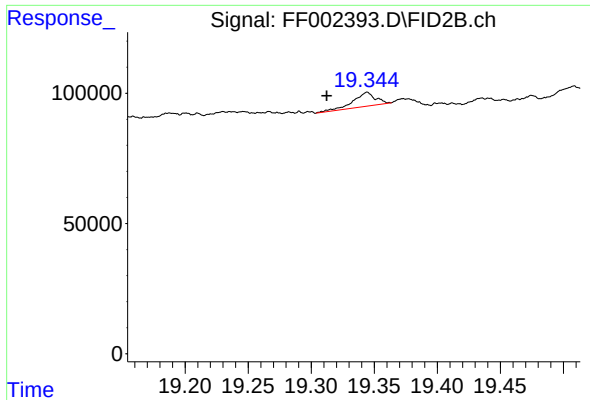


#15 N-TETRATRIACONTANE

R.T.: 19.344 min

Delta R.T.: 0.032 min

Response: 66410

Conc: 0.48 ug/ml

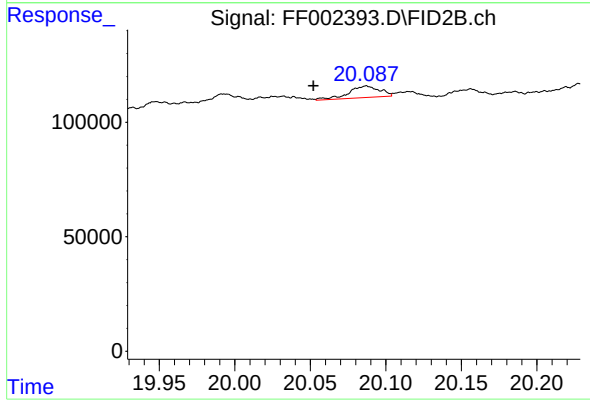

#16 N-HEXATRIACONTANE

R.T.: 20.087 min

Delta R.T.: 0.035 min

Response: 71941

Conc: 0.56 ug/ml