

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101018\
 Data File : FF002388.D
 Signal(s) : FID2B.ch
 Acq On : 10 Oct 2018 10:47
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 11 02:11:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.661	6240716	43.757 ug/ml
Target Compounds			
2) N-DECANE	4.390	8074405	49.846 ug/ml
3) N-DODECANE	6.414	8117926	49.348 ug/ml
4) N-TETRADECANE	8.207	8112555	48.702 ug/ml
5) N-HEXADECANE	9.809	8055944	48.103 ug/ml
6) N-OCTADECANE	11.252	7953942	47.371 ug/ml
7) N-EICOSANE	12.563	7689027	46.427 ug/ml
8) N-DOCOSANE	13.761	7397551	45.336 ug/ml
10) N-TETRACOSANE	14.866	7090472	44.343 ug/ml
11) N-HEXACOSANE	15.887	6826836	43.587 ug/ml
12) N-OCTACOSANE	16.839	6645604	43.444 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101018\
Data File : FF002388.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2018 10:47
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 11 02:11:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

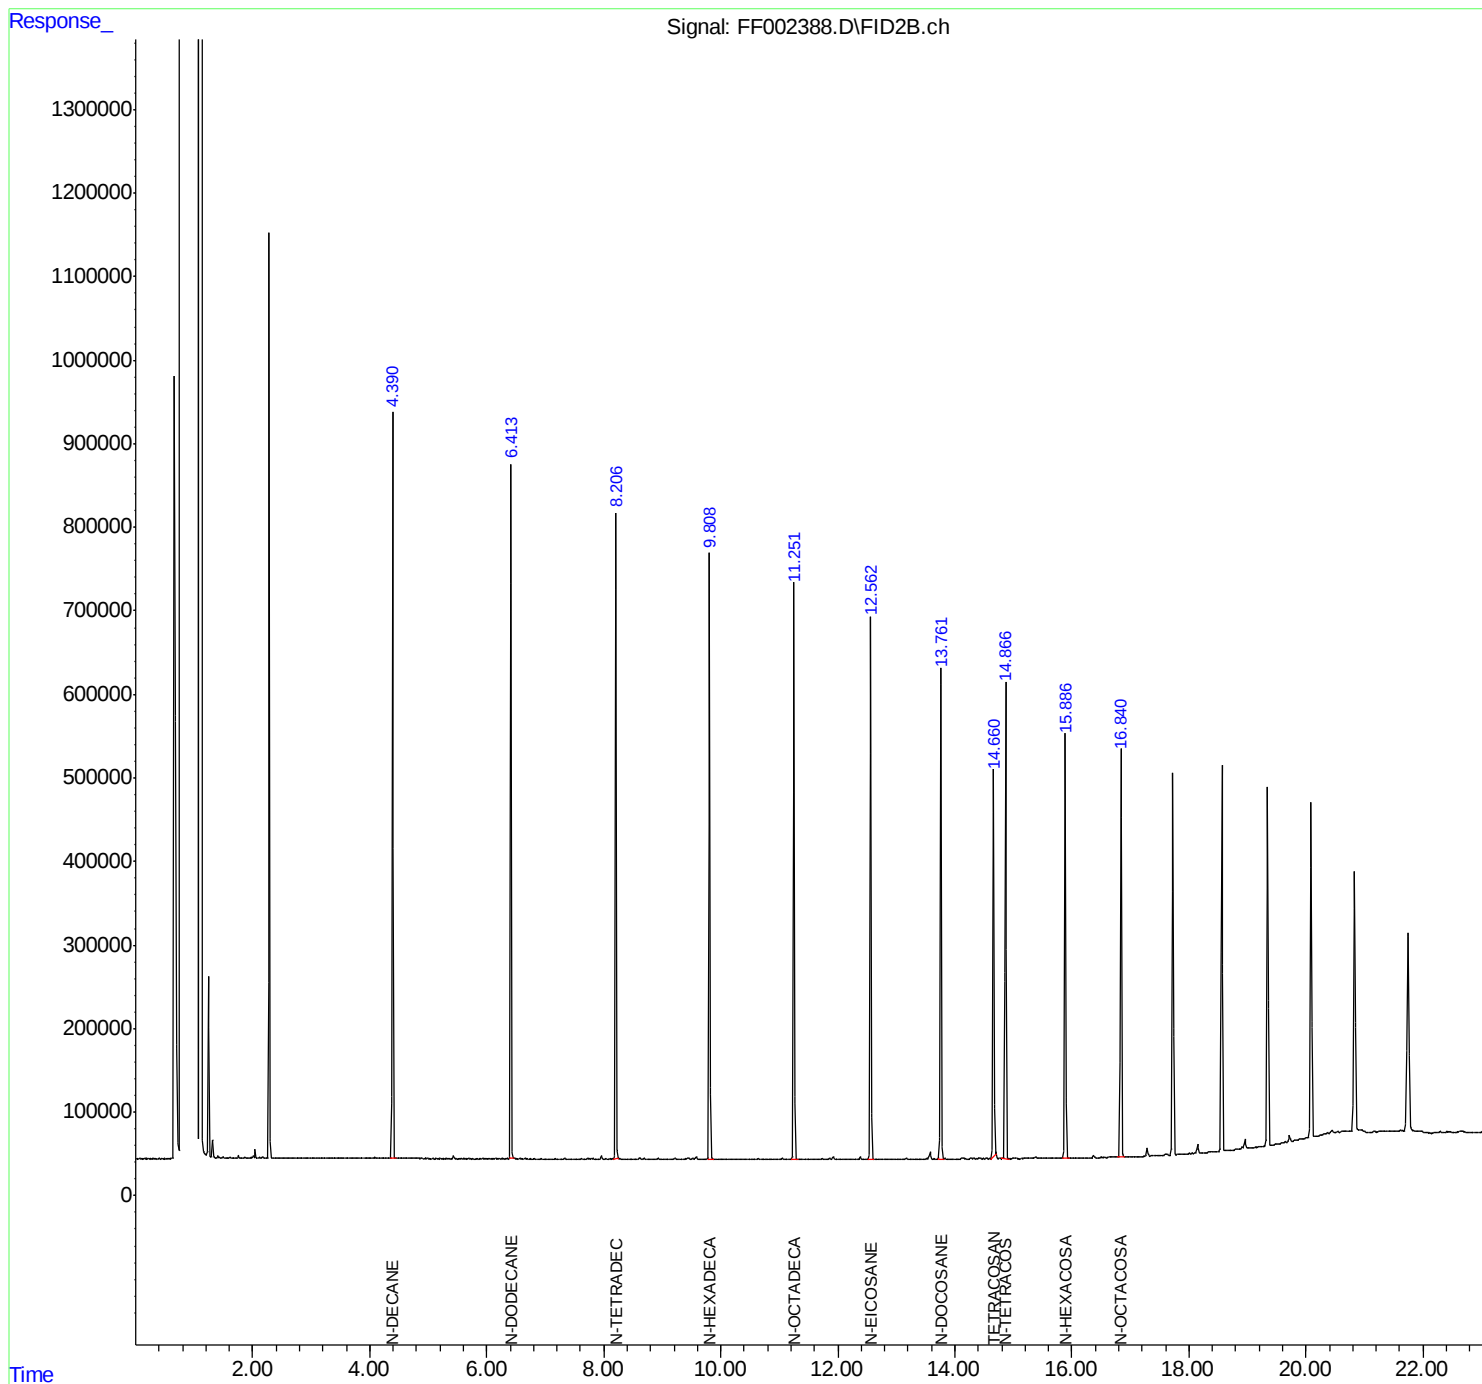

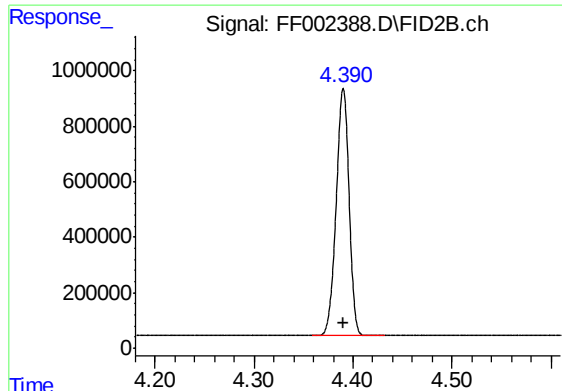


#2 N-DECANE

R.T.: 4.390 min
Delta R.T.: 0.000 min
Response: 8074405
Conc: 49.85 ug/ml

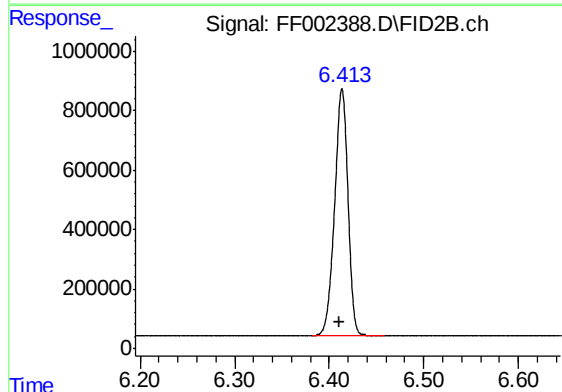


#3 N-DODECANE

R.T.: 6.414 min
Delta R.T.: 0.003 min
Response: 8117926
Conc: 49.35 ug/ml

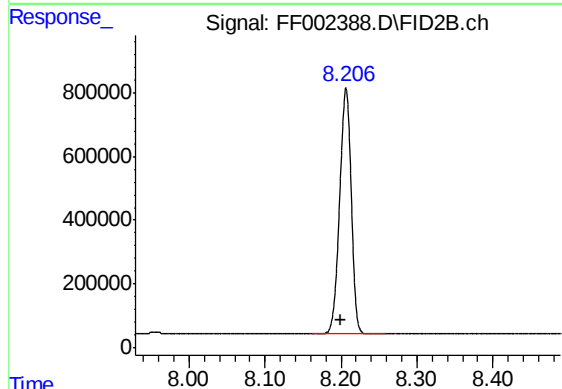


#4 N-TETRADECANE

R.T.: 8.207 min
Delta R.T.: 0.006 min
Response: 8112555
Conc: 48.70 ug/ml

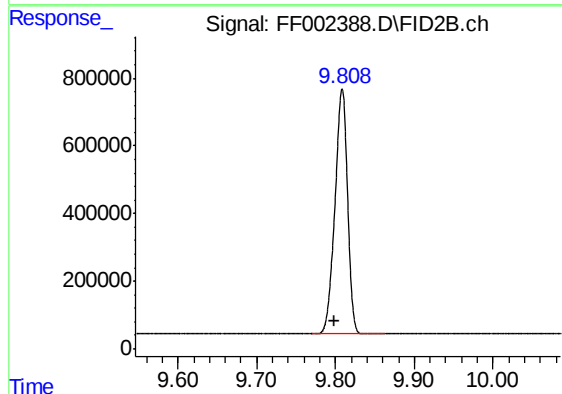


#5 N-HEXADECANE

R.T.: 9.809 min
Delta R.T.: 0.010 min
Response: 8055944
Conc: 48.10 ug/ml

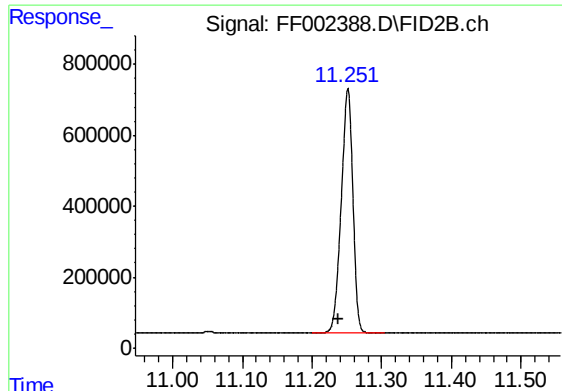


#6 N-OCTADECANE

R.T.: 11.252 min
Delta R.T.: 0.013 min
Response: 7953942
Conc: 47.37 ug/ml

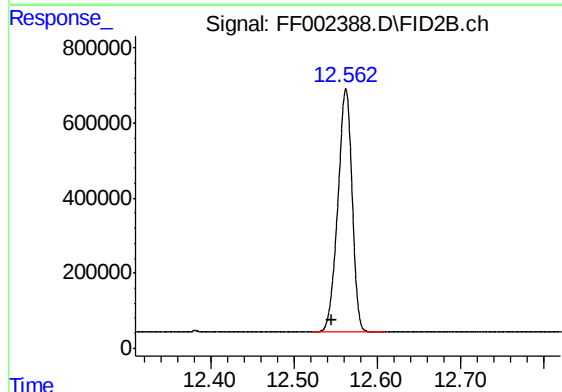


#7 N-EICOSANE

R.T.: 12.563 min
Delta R.T.: 0.016 min
Response: 7689027
Conc: 46.43 ug/ml

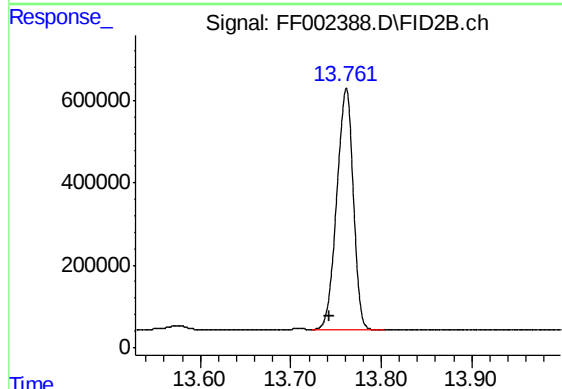


#8 N-DOCOSANE

R.T.: 13.761 min
Delta R.T.: 0.019 min
Response: 7397551
Conc: 45.34 ug/ml

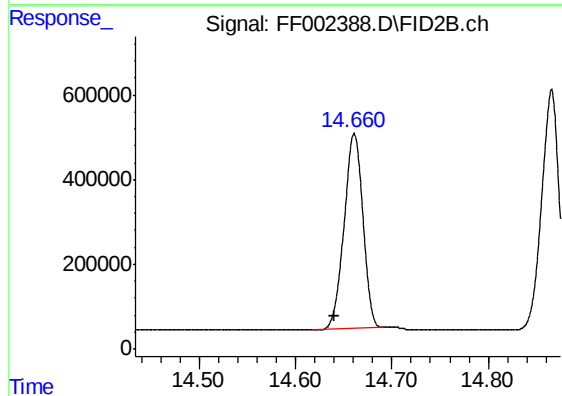


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.661 min
Delta R.T.: 0.020 min
Response: 6240716
Conc: 43.76 ug/ml

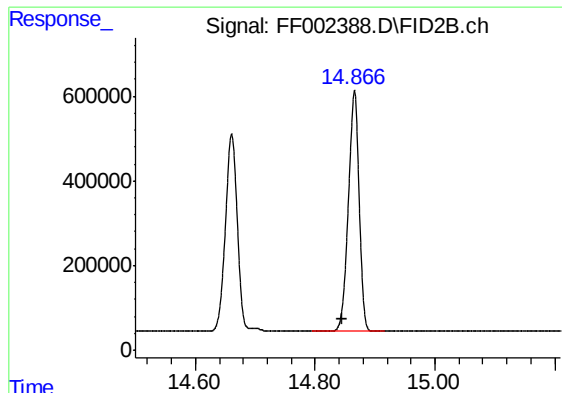


#10 N-TETRACOSANE

R.T.: 14.866 min
Delta R.T.: 0.021 min
Response: 7090472
Conc: 44.34 ug/ml

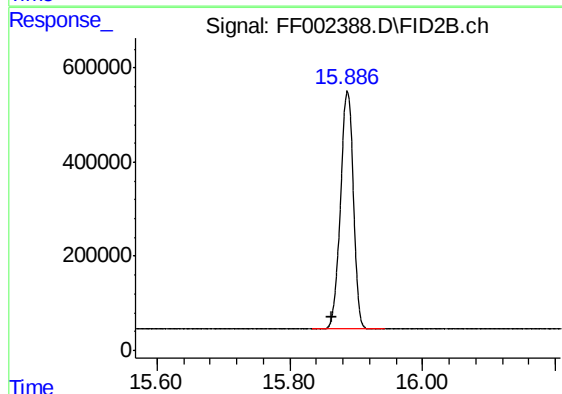

#11 N-HEXACOSANE

R.T.: 15.887 min
Delta R.T.: 0.023 min
Response: 6826836
Conc: 43.59 ug/ml

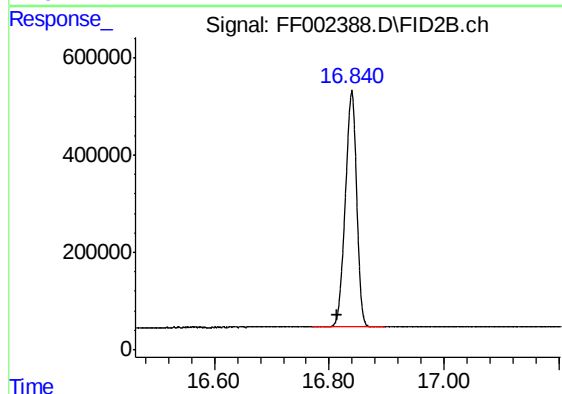

#12 N-OCTACOSANE

R.T.: 16.839 min
Delta R.T.: 0.027 min
Response: 6645604
Conc: 43.44 ug/ml