

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101018\
 Data File : FF002390.D
 Signal(s) : FID2B.ch
 Acq On : 10 Oct 2018 13:35
 Operator : AJ\SJ
 Sample : PB113696BS
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 11 02:00:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.656	1905015	13.357 ug/ml
Target Compounds			
2) N-DECANE	4.372	2529371	15.615 ug/ml
3) N-DODECANE	6.396	2613756	15.889 ug/ml
4) N-TETRADECANE	8.193	2609087	15.663 ug/ml
5) N-HEXADECANE	9.797	2596059	15.501 ug/ml
6) N-OCTADECANE	11.241	2592836	15.442 ug/ml
7) N-EICOSANE	12.553	2495230	15.066 ug/ml
8) N-DOCOSANE	13.754	2427424	14.876 ug/ml
10) N-TETRACOSANE	14.859	2337119	14.616 ug/ml
11) N-HEXACOSANE	15.882	2241305	14.310 ug/ml
12) N-OCTACOSANE	16.835	2165721	14.158 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101018\
Data File : FF002390.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2018 13:35
Operator : AJ\SJ
Sample : PB113696BS
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 11 02:00:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

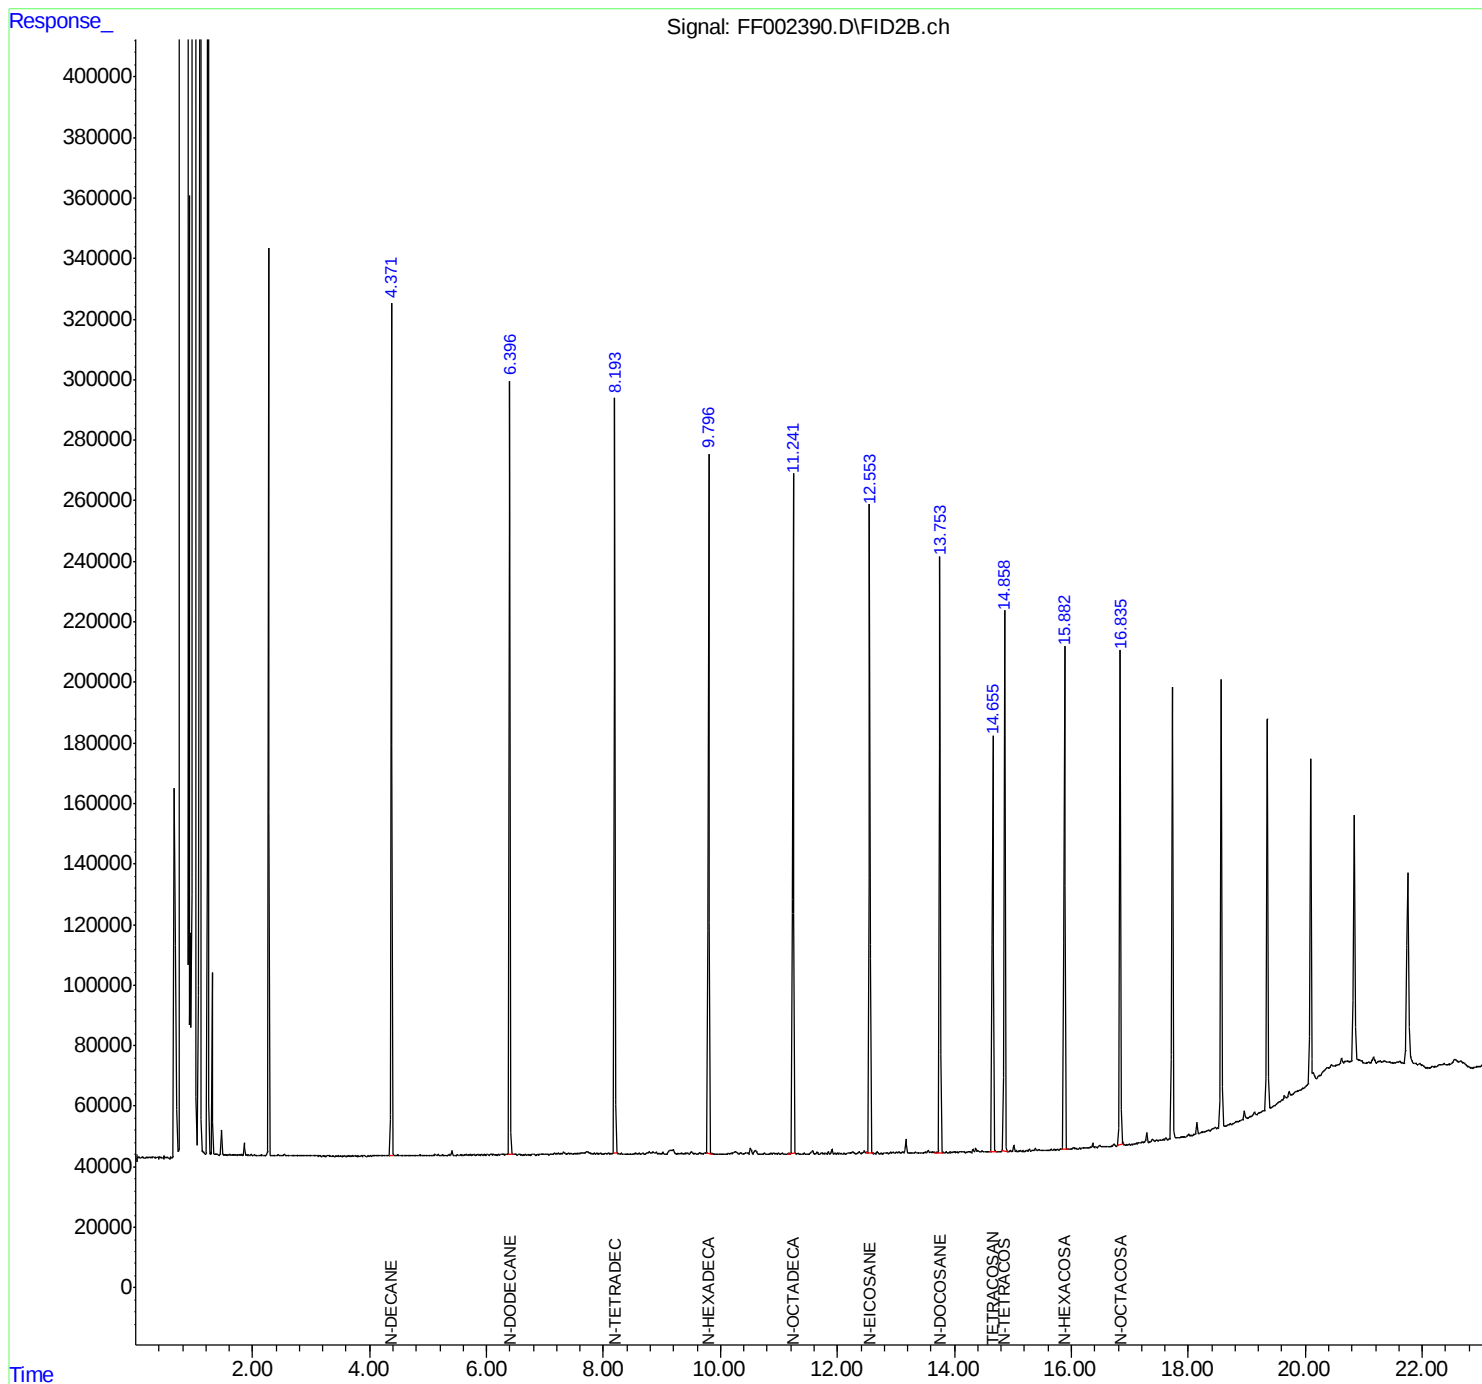

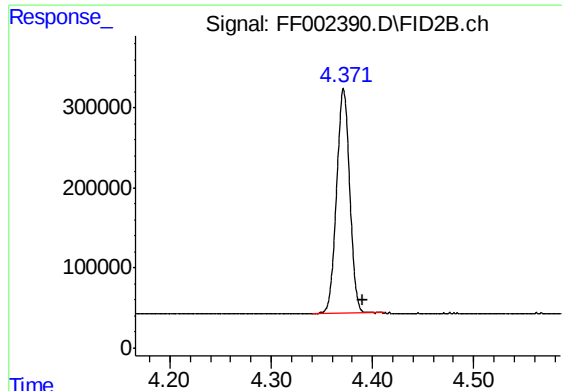


#2 N-DECANE

R.T.: 4.372 min
Delta R.T.: -0.019 min
Response: 2529371
Conc: 15.61 ug/ml

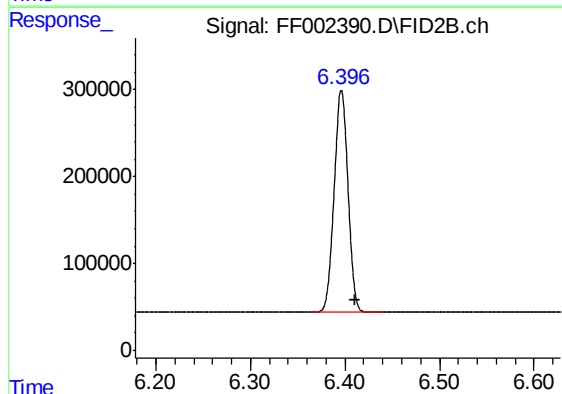


#3 N-DODECANE

R.T.: 6.396 min
Delta R.T.: -0.014 min
Response: 2613756
Conc: 15.89 ug/ml

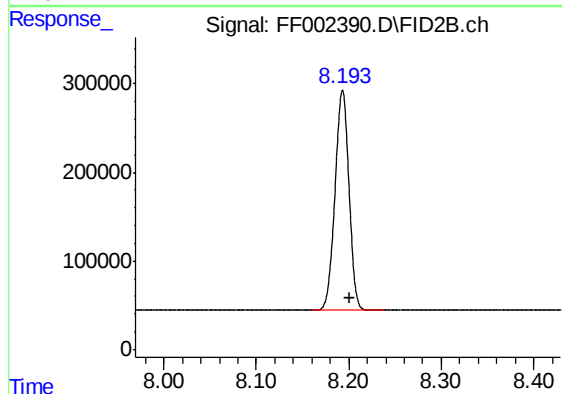


#4 N-TETRADECANE

R.T.: 8.193 min
Delta R.T.: -0.007 min
Response: 2609087
Conc: 15.66 ug/ml

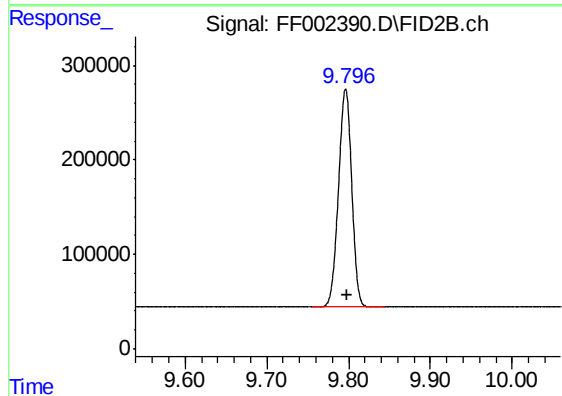


#5 N-HEXADECANE

R.T.: 9.797 min
Delta R.T.: -0.002 min
Response: 2596059
Conc: 15.50 ug/ml

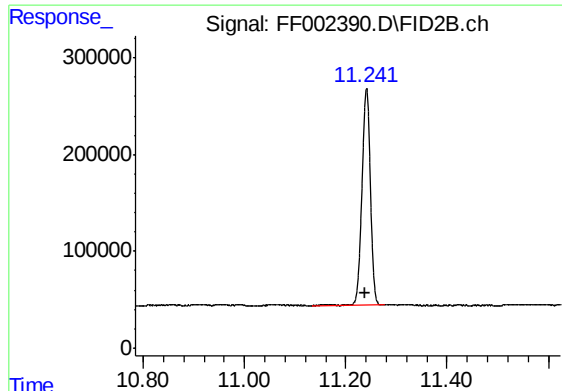


#6 N-OCTADECANE

R.T.: 11.241 min
Delta R.T.: 0.003 min
Response: 2592836
Conc: 15.44 ug/ml

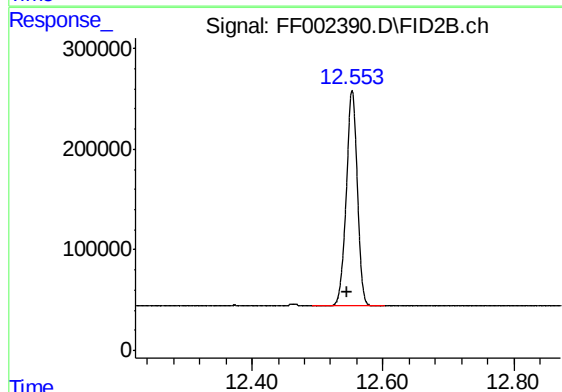


#7 N-EICOSANE

R.T.: 12.553 min
Delta R.T.: 0.007 min
Response: 2495230
Conc: 15.07 ug/ml

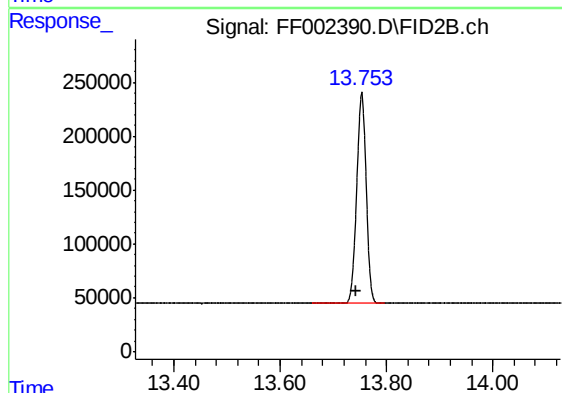


#8 N-DOCOSANE

R.T.: 13.754 min
Delta R.T.: 0.011 min
Response: 2427424
Conc: 14.88 ug/ml

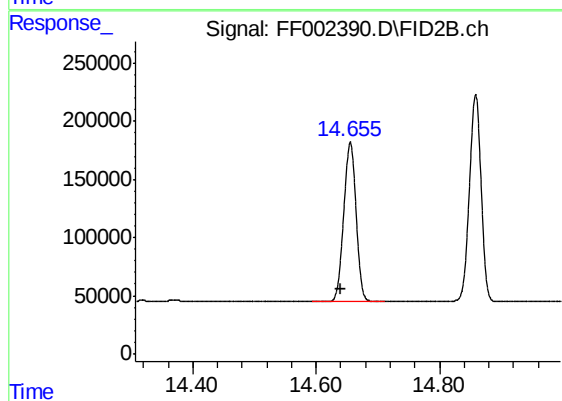


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.656 min
Delta R.T.: 0.015 min
Response: 1905015
Conc: 13.36 ug/ml

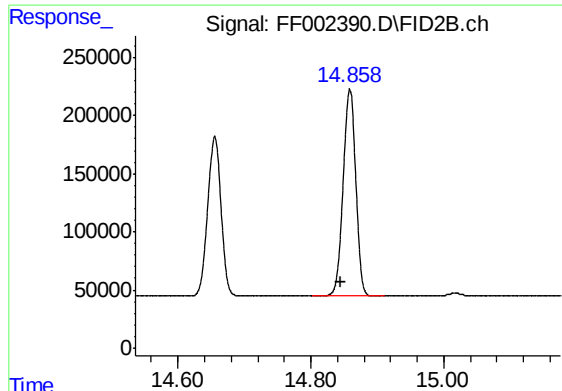


#10 N-TETRACOSANE

R.T.: 14.859 min
Delta R.T.: 0.014 min
Response: 2337119
Conc: 14.62 ug/ml

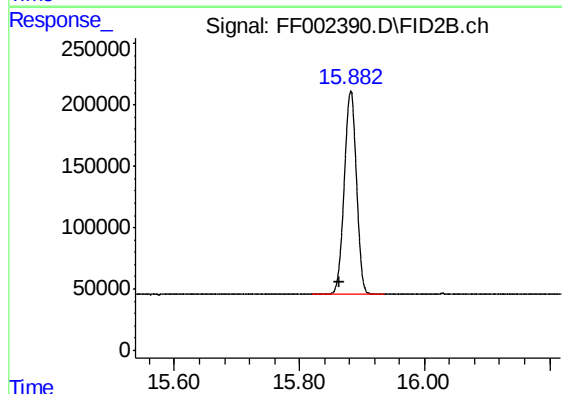

#11 N-HEXACOSANE

R.T.: 15.882 min
Delta R.T.: 0.019 min
Response: 2241305
Conc: 14.31 ug/ml

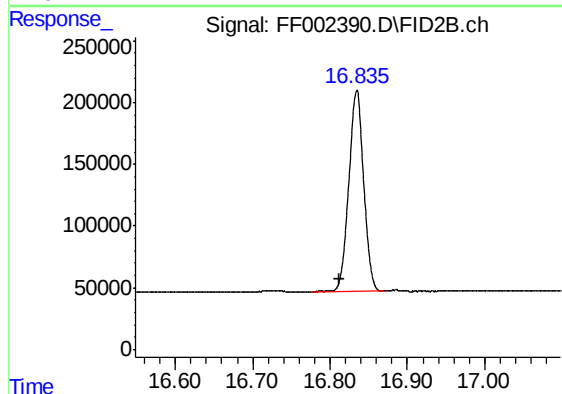

#12 N-OCTACOSANE

R.T.: 16.835 min
Delta R.T.: 0.023 min
Response: 2165721
Conc: 14.16 ug/ml