

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101023AL\
Data File : FF013590.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2023 08:03
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 01:58:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100623.M
Quant Title : GC Extractables
QLast Update : Sat Oct 07 07:01:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.884	223057	1.624 ug/ml
20) T	n-Hexatriacontane (C36)	20.434	270214	2.167 ug/ml
22) T	n-Tetracontane (C40)	22.059f	254933	2.216 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101023AL\
Data File : FF013590.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2023 08:03
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 01:58:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100623.M
Quant Title : GC Extractables
QLast Update : Sat Oct 07 07:01:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

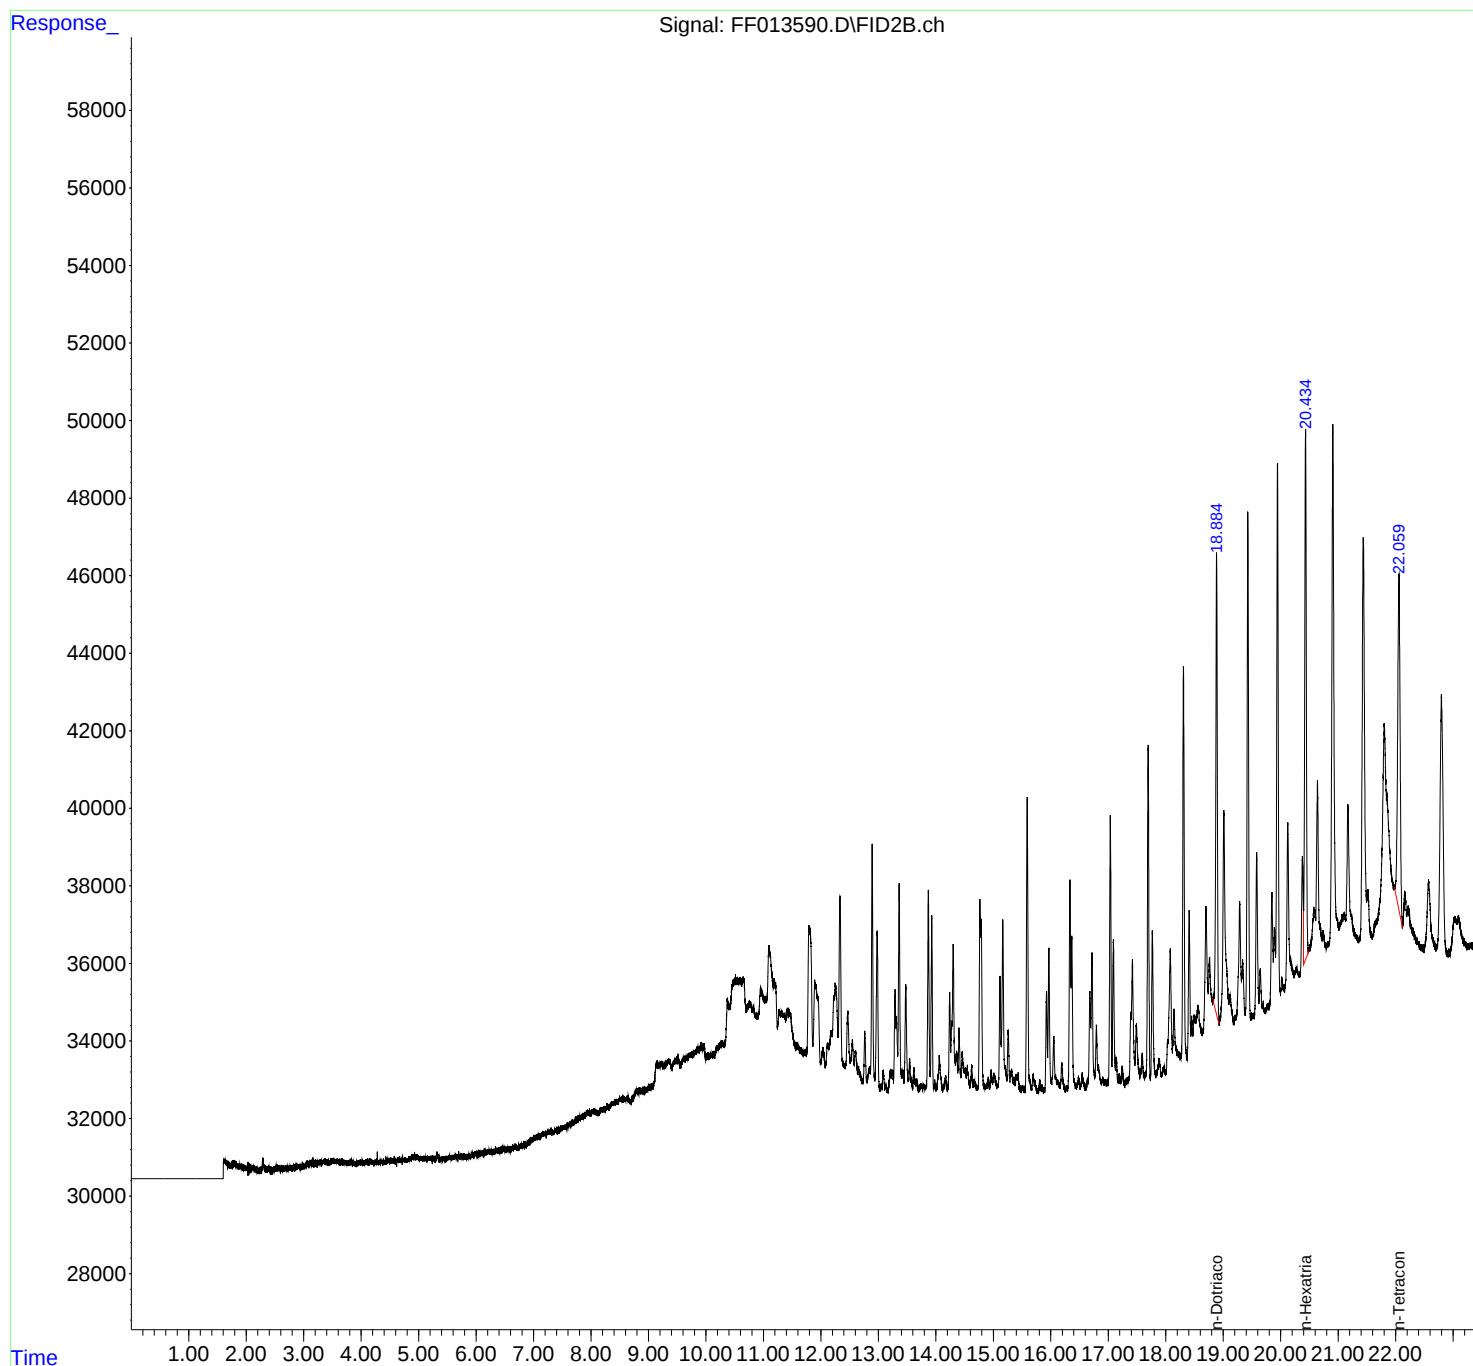


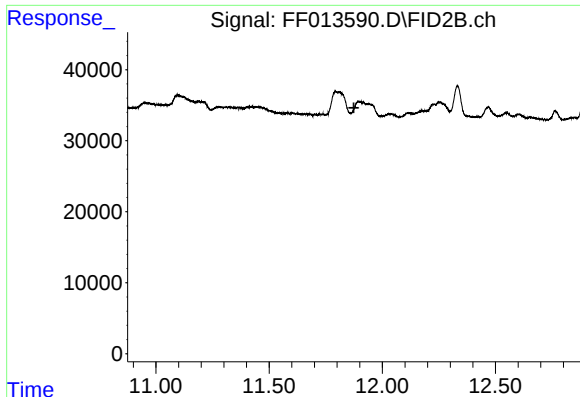

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.875 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

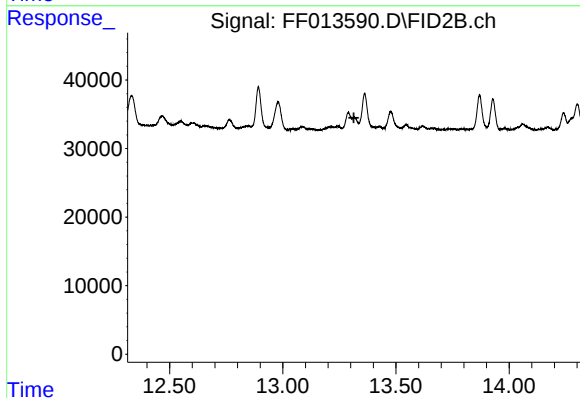


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.314 min
Response: 0
Conc: N.D.

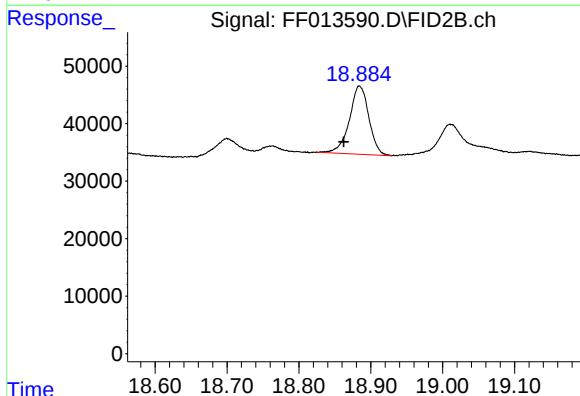


#18 n-Dotriacontane (C32)

R.T.: 18.884 min
Delta R.T.: 0.022 min
Response: 223057
Conc: 1.62 ug/ml

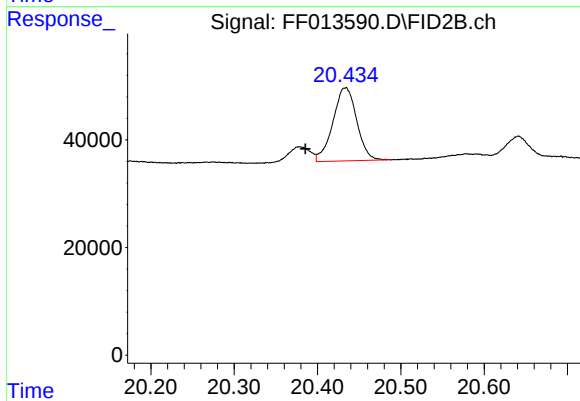

#20 n-Hexatriacontane (C36)

R.T.: 20.434 min
Delta R.T.: 0.048 min
Response: 270214
Conc: 2.17 ug/ml

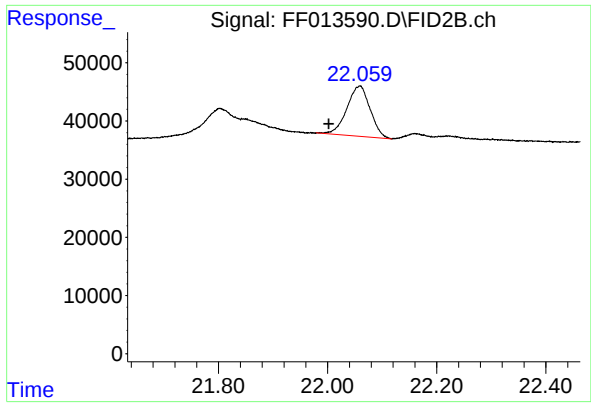

#22 n-Tetracontane (C40)

R.T.: 22.059 min
Delta R.T.: 0.056 min
Response: 254933
Conc: 2.22 ug/ml

Instrument :

FID_F

ClientSampleId :