

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101023AL\
 Data File : FF013594.D
 Signal(s) : FID2B.ch
 Acq On : 10 Oct 2023 10:05
 Operator : YP\AJ
 Sample : PB156130BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 11 01:59:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100623.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 07 07:01:38 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.314	6520926	54.411 ug/ml
Spiked Amount 50.000		Recovery =	108.82%
Target Compounds			
4) T n-Dodecane (C12)	6.683	68103	0.525 ug/ml
13) T n-Docosane (C22)	14.066	97639	0.724 ug/ml
14) T n-Tetracosane (C24)	15.169	204969	1.500 ug/ml
15) T n-Hexacosane (C26)	16.190	264586	1.943 ug/ml
16) T n-Octacosane (C28)	17.140	342161	2.559 ug/ml
17) T n-Tricontane (C30)	18.027	421210	3.040 ug/ml
18) T n-Dotriacontane (C32)	18.860	416280	3.030 ug/ml
19) T n-Tetratriacontane (C34)	19.642	227337	1.755 ug/ml
20) T n-Hexatriacontane (C36)	20.382	132024	1.059 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101023AL\
Data File : FF013594.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2023 10:05
Operator : YP\AJ
Sample : PB156130BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 01:59:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100623.M
Quant Title : GC Extractables
QLast Update : Sat Oct 07 07:01:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

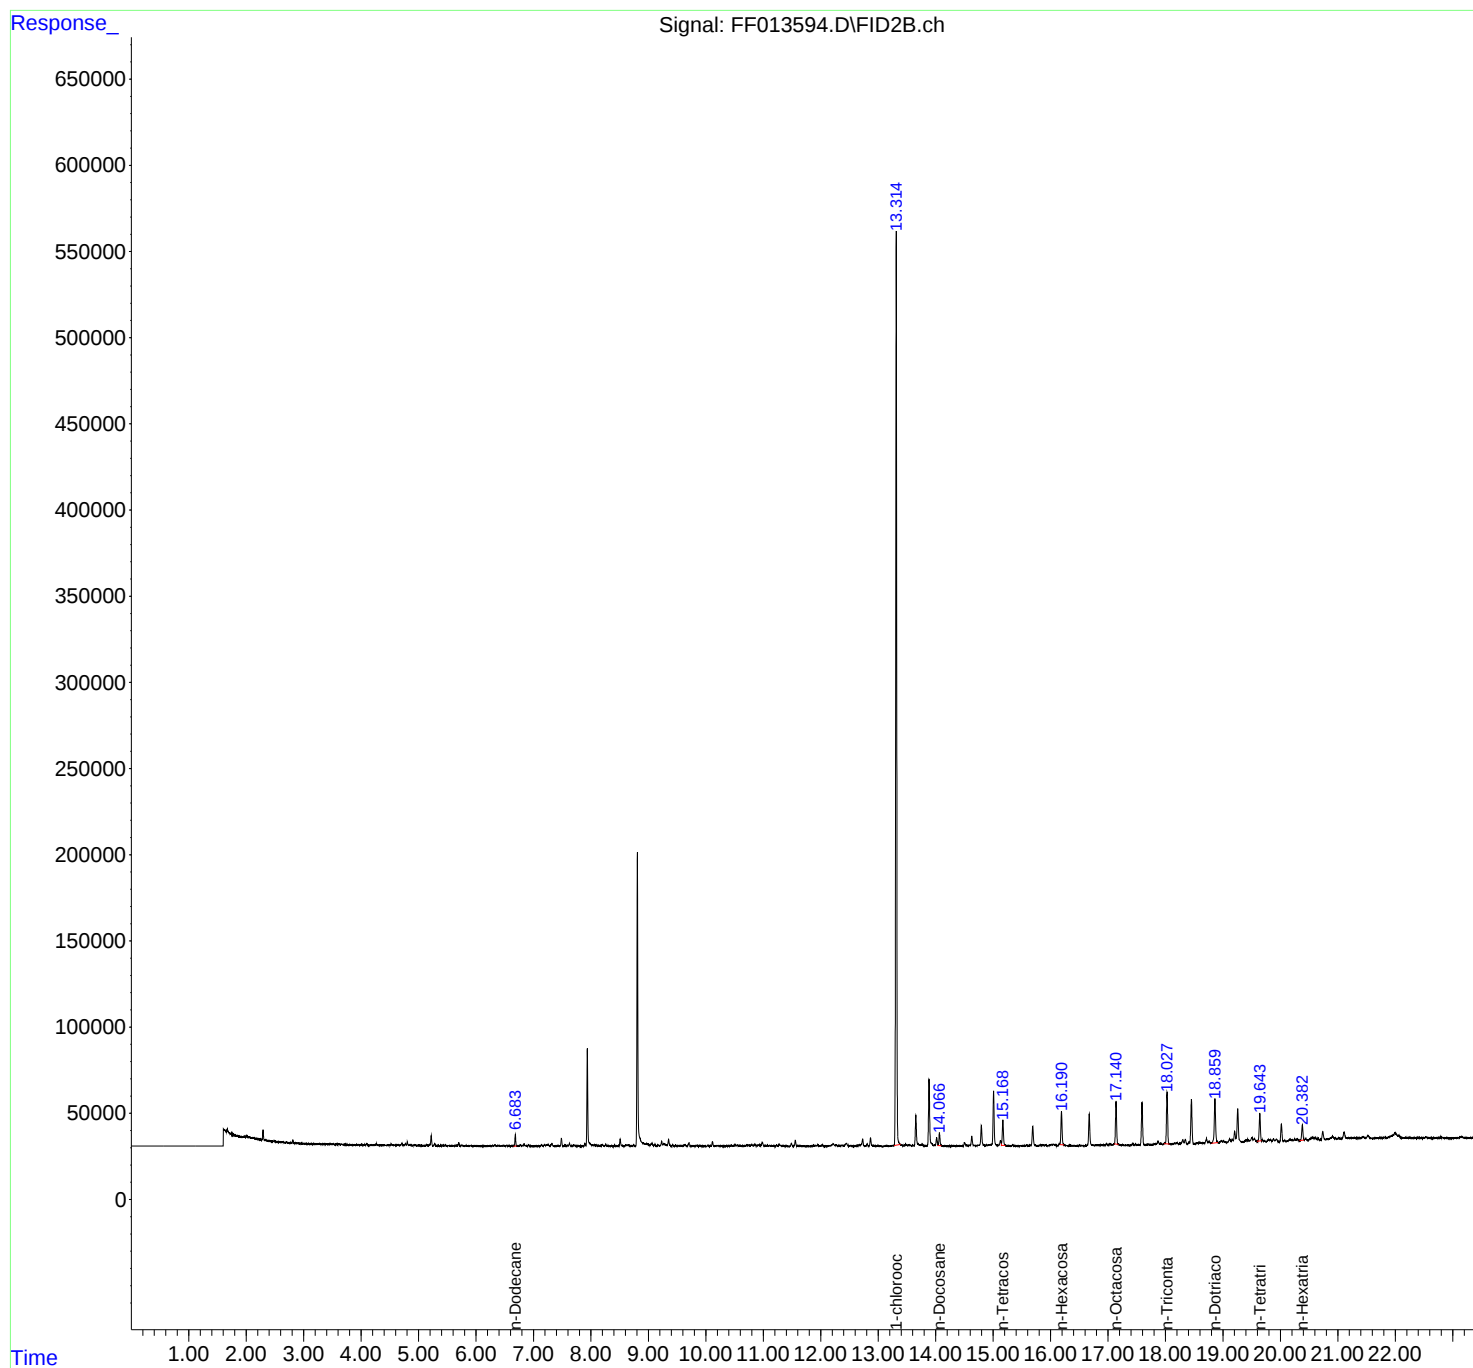


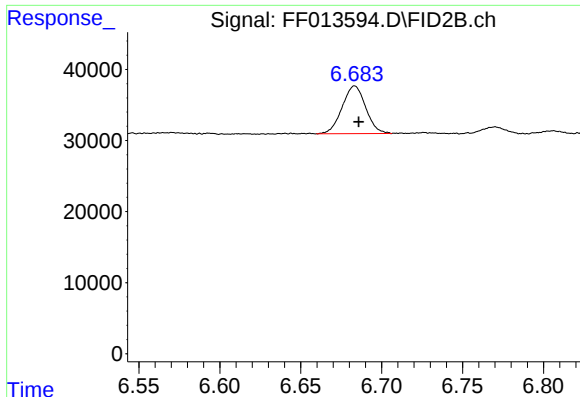

#4 n-Dodecane (C12)


R.T.: 6.683 min
Delta R.T.: -0.003 min
Response: 68103
Conc: 0.52 ug/ml

Instrument :
FID_F
ClientSampleId :

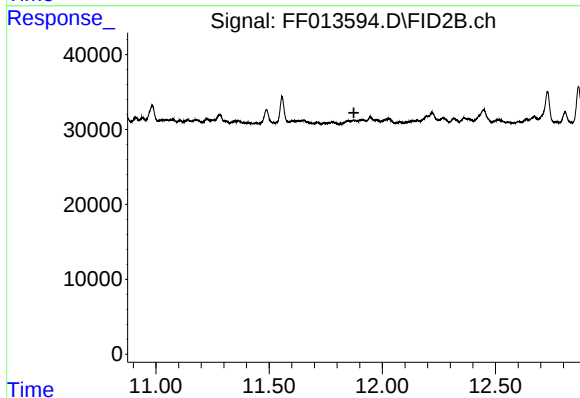


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.875 min
Response: 0
Conc: N.D.

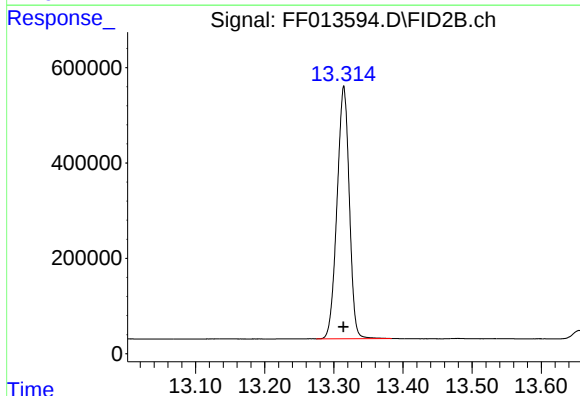


#12 1-chlorooctadecane (SURR)

R.T.: 13.314 min
Delta R.T.: 0.000 min
Response: 6520926
Conc: 54.41 ug/ml

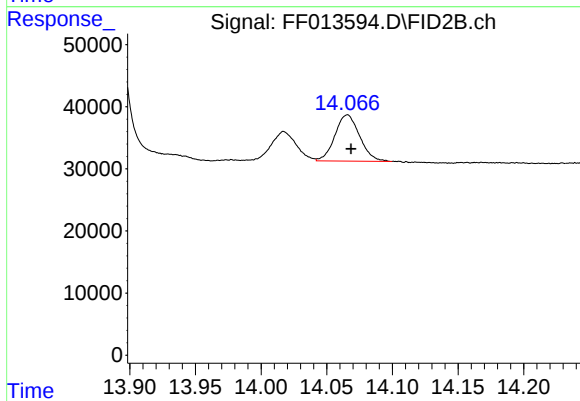

#13 n-Docosane (C22)


R.T.: 14.066 min
Delta R.T.: -0.003 min
Response: 97639
Conc: 0.72 ug/ml

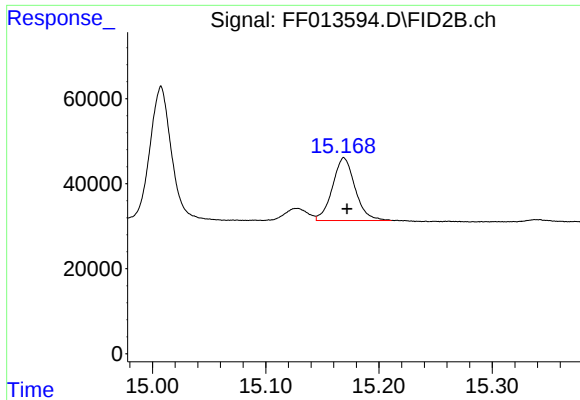

#14 n-Tetracosane (C24)


R.T.: 15.169 min
Delta R.T.: -0.003 min
Response: 204969
Conc: 1.50 ug/ml

Instrument :
FID_F
ClientSampleId :

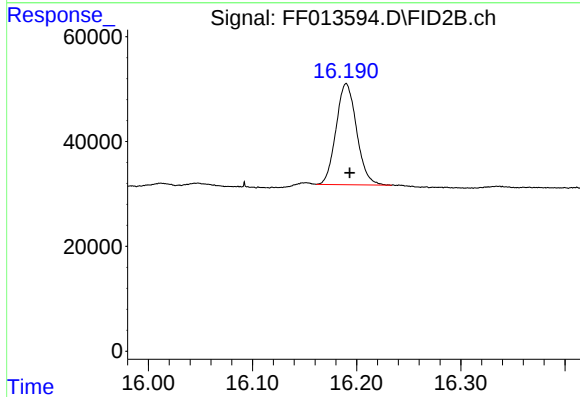


#15 n-Hexacosane (C26)

R.T.: 16.190 min
Delta R.T.: -0.003 min
Response: 264586
Conc: 1.94 ug/ml

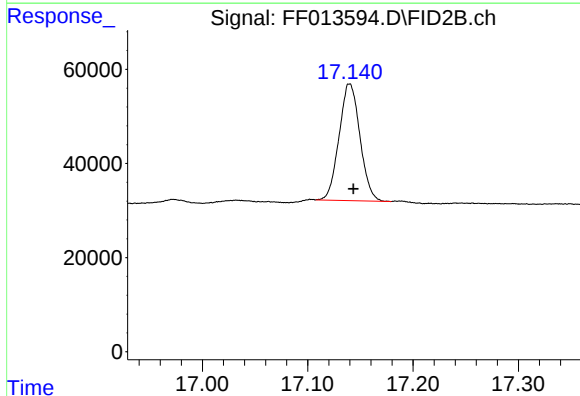


#16 n-Octacosane (C28)

R.T.: 17.140 min
Delta R.T.: -0.004 min
Response: 342161
Conc: 2.56 ug/ml

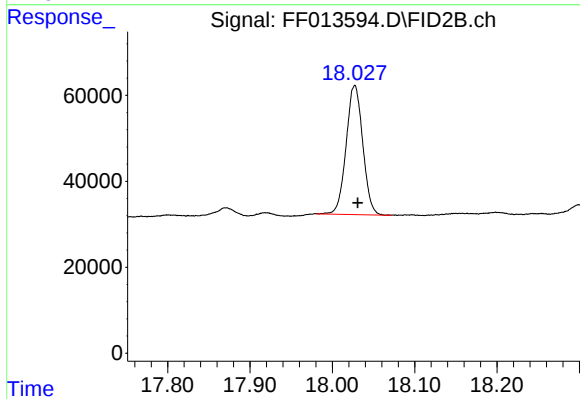

#17 n-Tricontane (C30)


R.T.: 18.027 min
Delta R.T.: -0.004 min
Response: 421210
Conc: 3.04 ug/ml

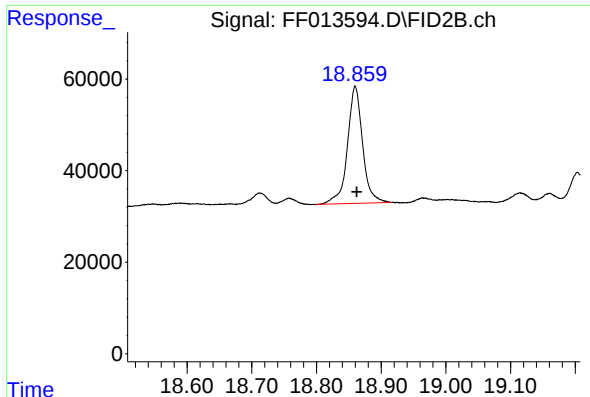

#18 n-Dotriacontane (C32)


R.T.: 18.860 min
Delta R.T.: -0.002 min
Response: 416280
Conc: 3.03 ug/ml

Instrument :
FID_F
ClientSampleId :

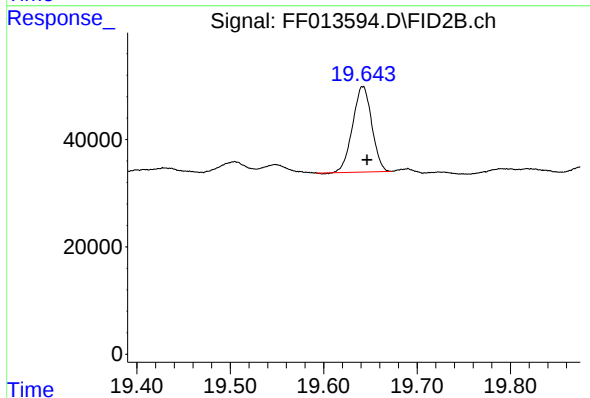

#19 n-Tetatriacontane (C34)

R.T.: 19.642 min
Delta R.T.: -0.005 min
Response: 227337
Conc: 1.76 ug/ml

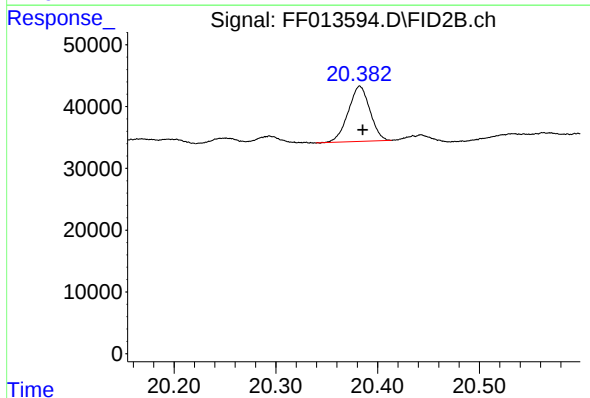

#20 n-Hexatriacontane (C36)

R.T.: 20.382 min
Delta R.T.: -0.003 min
Response: 132024
Conc: 1.06 ug/ml