

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF101024\  
Data File : FF014618.D  
Signal(s) : FID2B.ch  
Acq On : 10 Oct 2024 13:44  
Operator : YP\AJ  
Sample : PB164028BL  
Misc :  
ALS Vial : 61 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Oct 11 01:25:21 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF100324.M  
Quant Title :  
QLast Update : Thu Oct 03 12:23:07 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.883 | 2138174  | 16.349 ug/ml |
| Target Compounds              |        |          |              |
| 13) N-TRIACONTANE             | 17.950 | 88059    | 0.603 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.783 | 105003   | 0.723 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.567 | 83187    | 0.604 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF101024\  
Data File : FF014618.D  
Signal(s) : FID2B.ch  
Acq On : 10 Oct 2024 13:44  
Operator : YP\AJ  
Sample : PB164028BL  
Misc :  
ALS Vial : 61 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Oct 11 01:25:21 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF100324.M  
Quant Title :  
QLast Update : Thu Oct 03 12:23:07 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

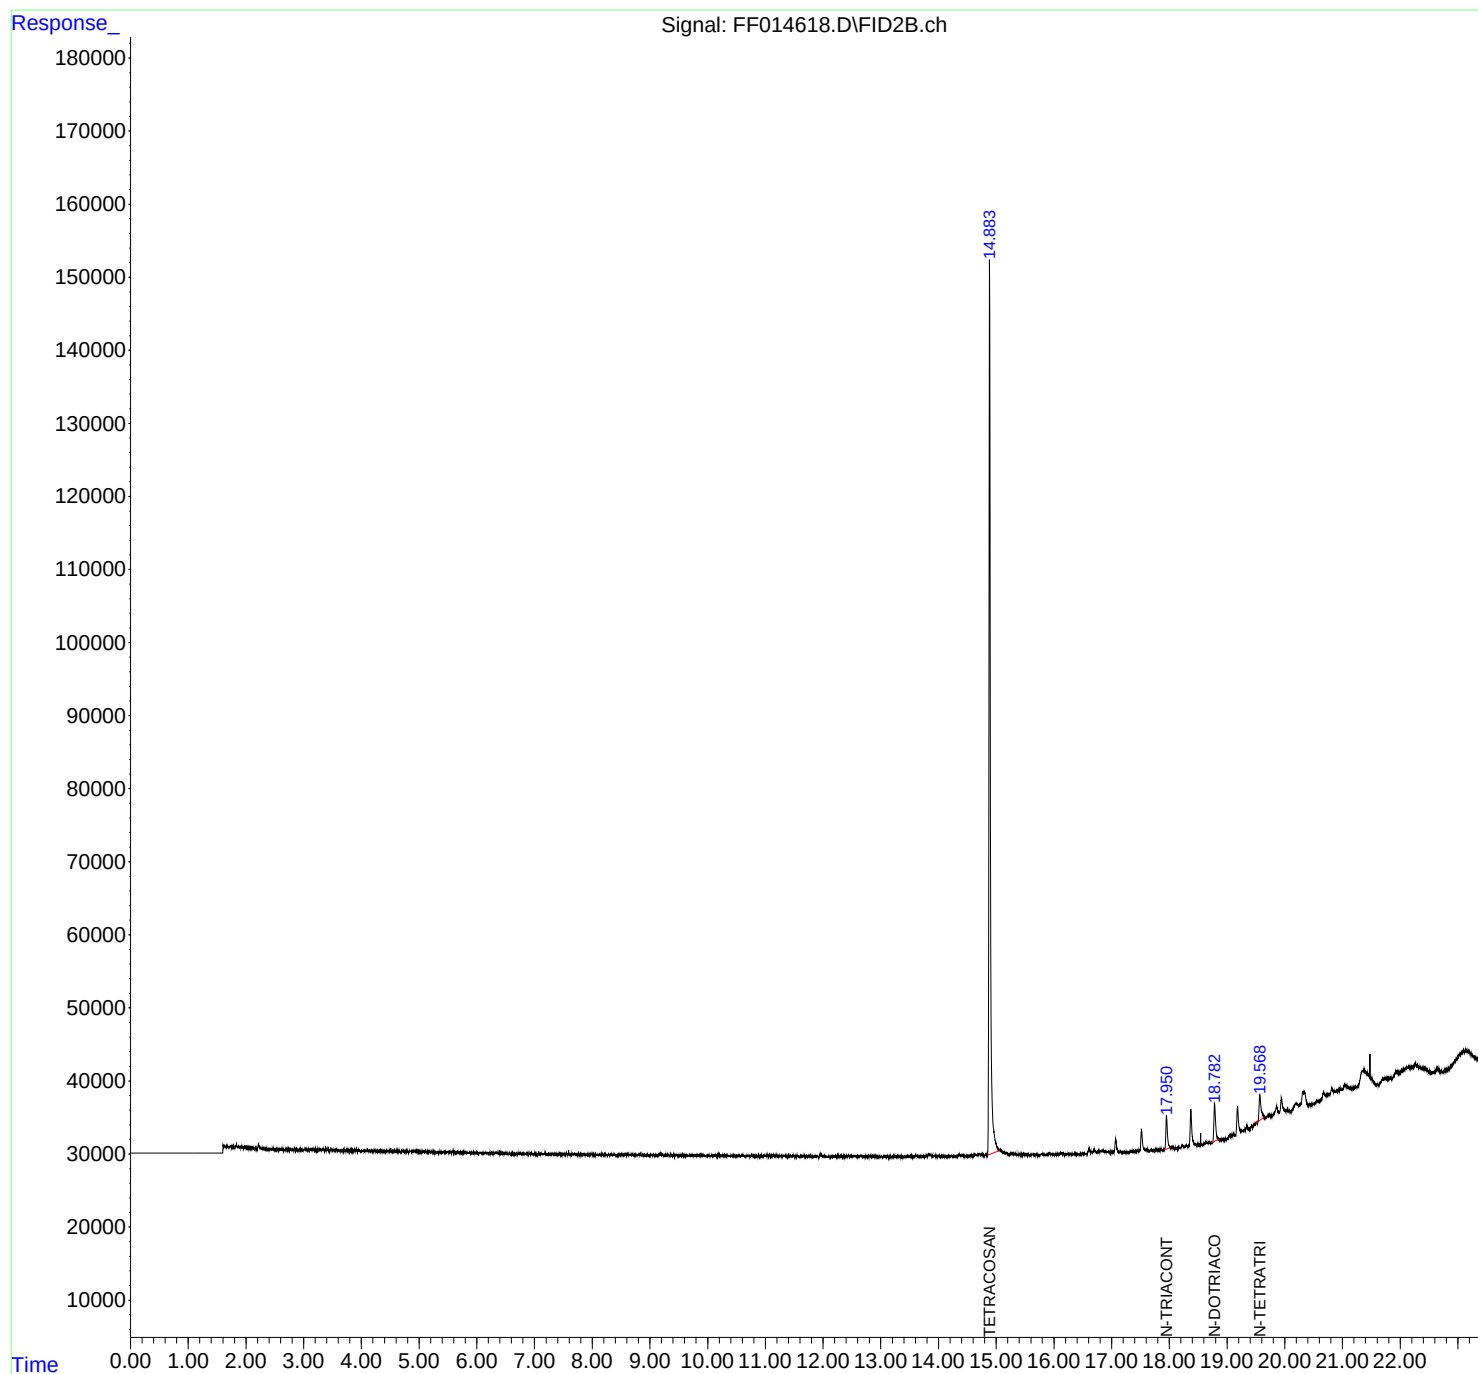


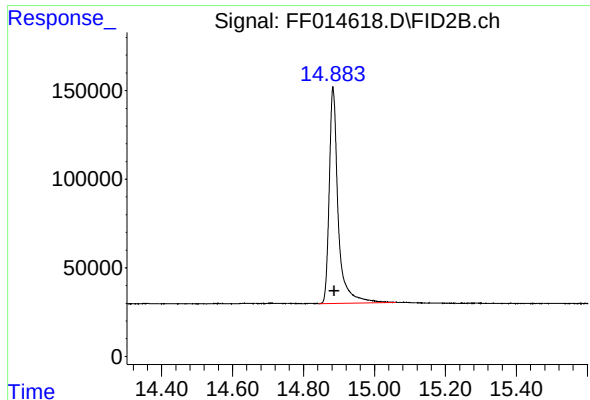

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.883 min  
Delta R.T.: -0.004 min  
Response: 2138174  
Conc: 16.35 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

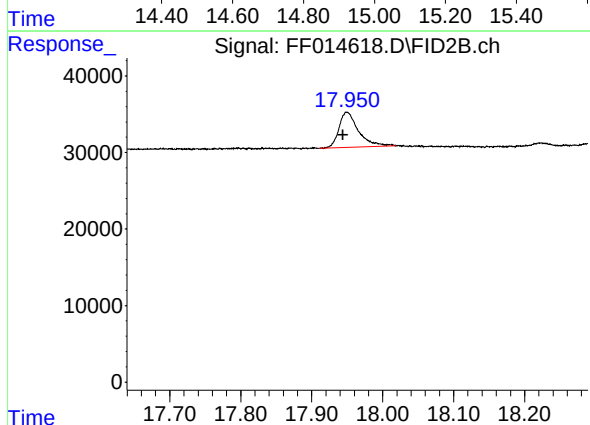


#13 N-TRIACONTANE

R.T.: 17.950 min  
Delta R.T.: 0.006 min  
Response: 88059  
Conc: 0.60 ug/ml

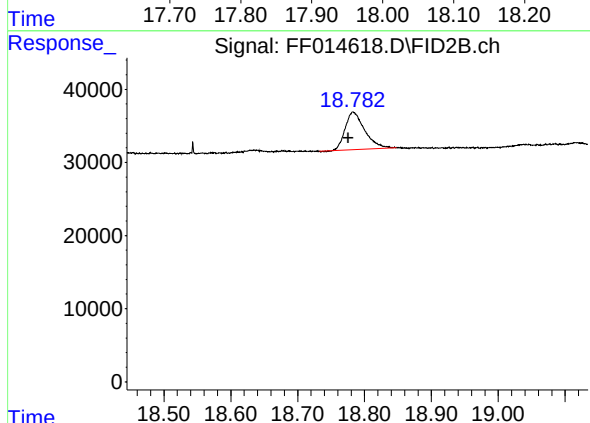

#14 N-DOTRIACONTANE

R.T.: 18.783 min  
Delta R.T.: 0.008 min  
Response: 105003  
Conc: 0.72 ug/ml

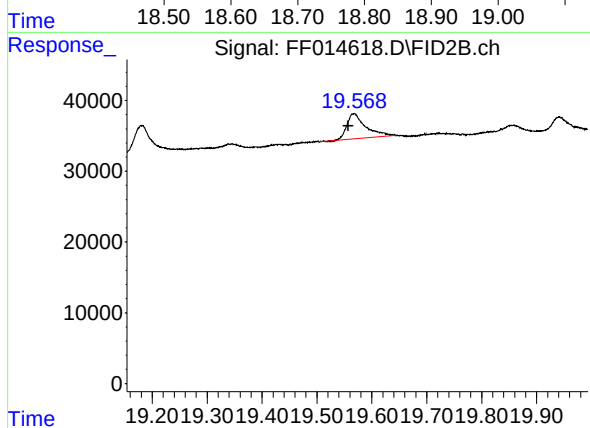

#15 N-TETRATRIACONTANE

R.T.: 19.567 min  
Delta R.T.: 0.010 min  
Response: 83187  
Conc: 0.60 ug/ml