

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101024\
Data File : FF014618.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2024 13:44
Operator : YP\AJ
Sample : PB164028BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB164028BL

Integration File: autoint1.e
Quant Time: Oct 11 01:25:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100324.M
Quant Title :
QLast Update : Thu Oct 03 12:23:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.883	2138174	16.349 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101024\
Data File : FF014618.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2024 13:44
Operator : YP\AJ
Sample : PB164028BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB164028BL

Integration File: autoint1.e
Quant Time: Oct 11 01:25:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100324.M
Quant Title :
QLast Update : Thu Oct 03 12:23:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

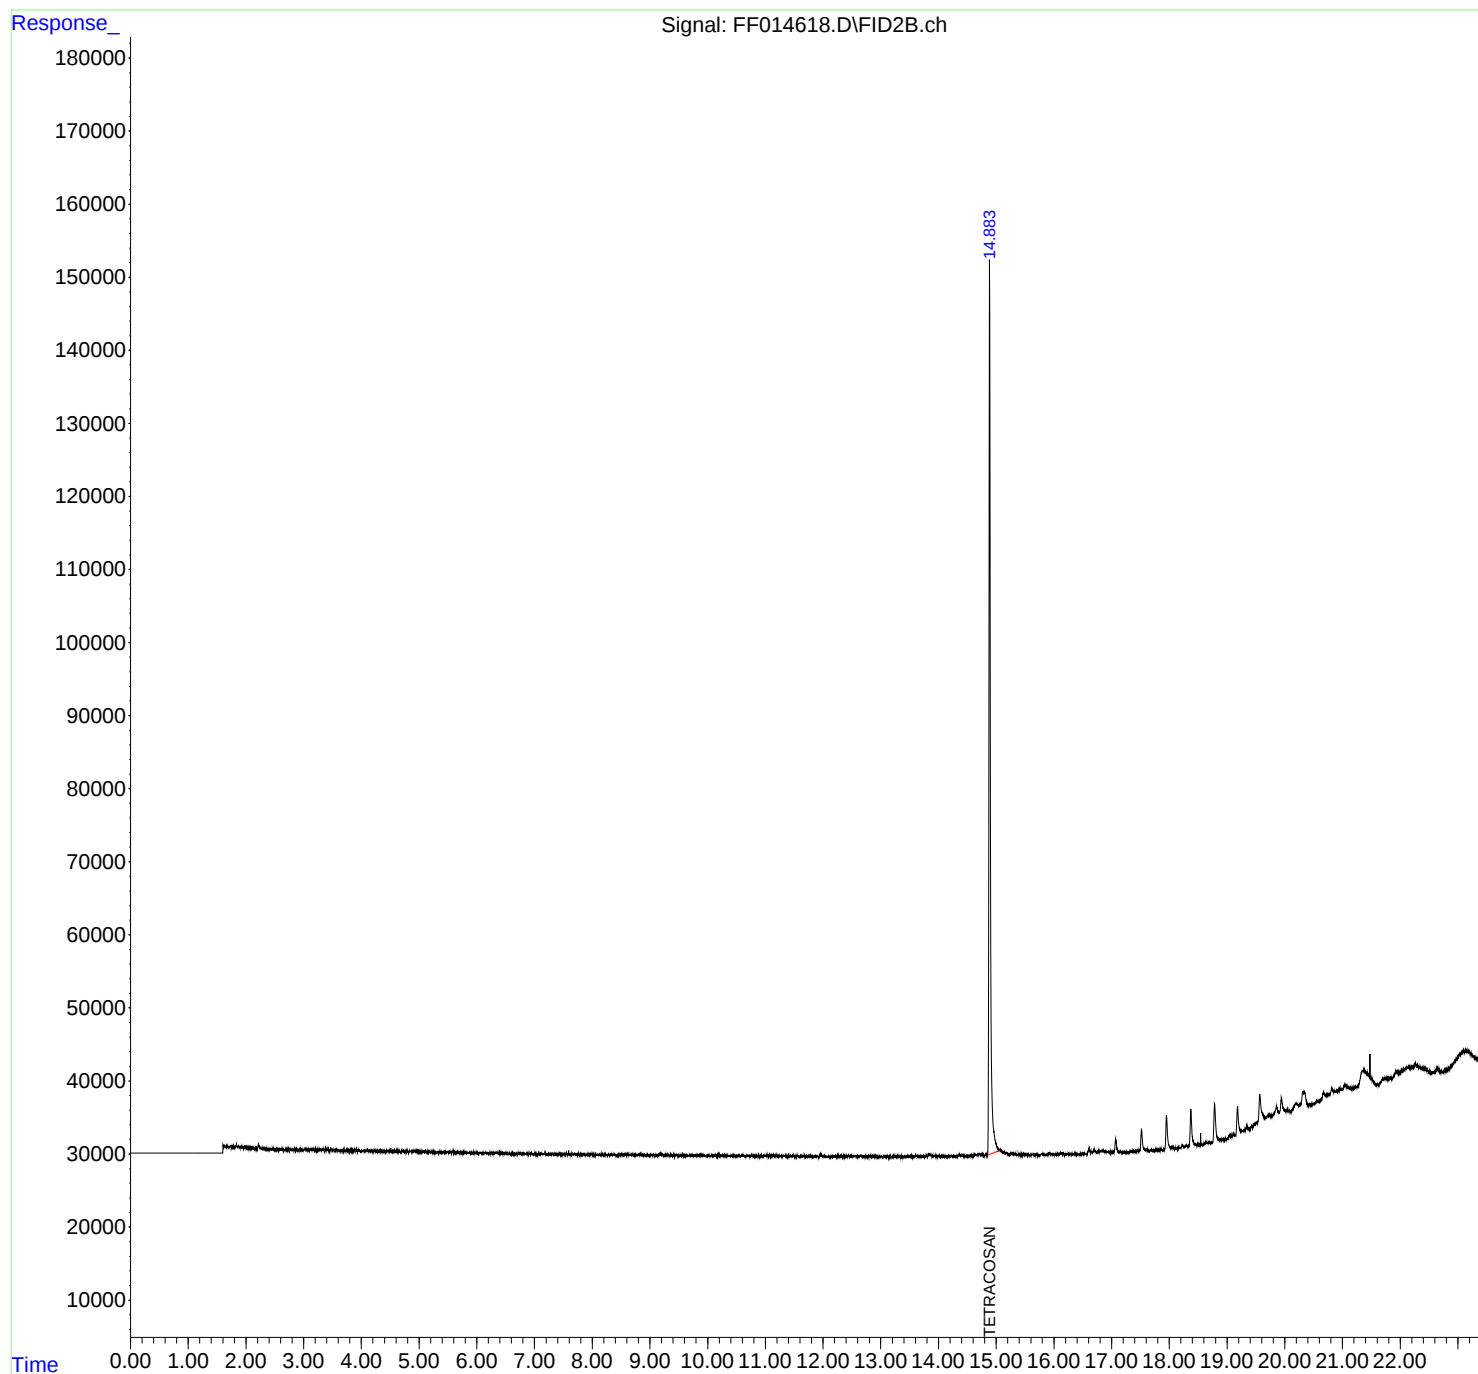

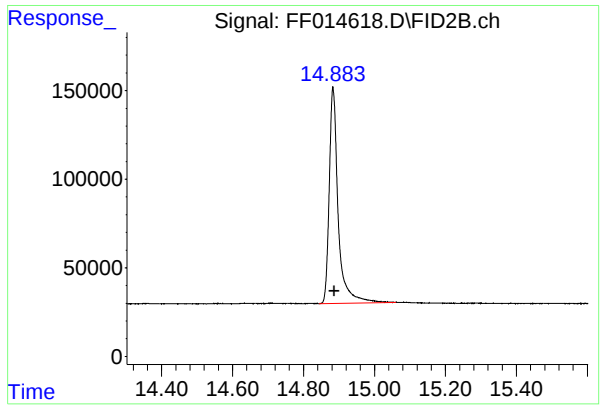

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.883 min
Delta R.T.: -0.004 min
Response: 2138174
Conc: 16.35 ug/ml

Instrument :
FID_F
ClientSampleId :
PB164028BL