

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101119\
 Data File : FF005782.D
 Signal(s) : FID2B.ch
 Acq On : 11 Oct 2019 10:53
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 11 22:27:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
 Quant Title :
 QLast Update : Thu Oct 03 04:07:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3)	N-DODECANE	6.429	5192049 32.969 ug/ml
12)	N-OCTACOSANE	16.845	4554026 31.976 ug/ml
13)	N-TRIACONTANE	17.731	506656 3.648 ug/ml
14)	N-DOTRIACONTANE	18.566	590136 4.404 ug/ml
15)	N-TETRATRIACONTANE	19.351	404729 3.347 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101119\
Data File : FF005782.D
Signal(s) : FID2B.ch
Acq On : 11 Oct 2019 10:53
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 22:27:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
Quant Title :
QLast Update : Thu Oct 03 04:07:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

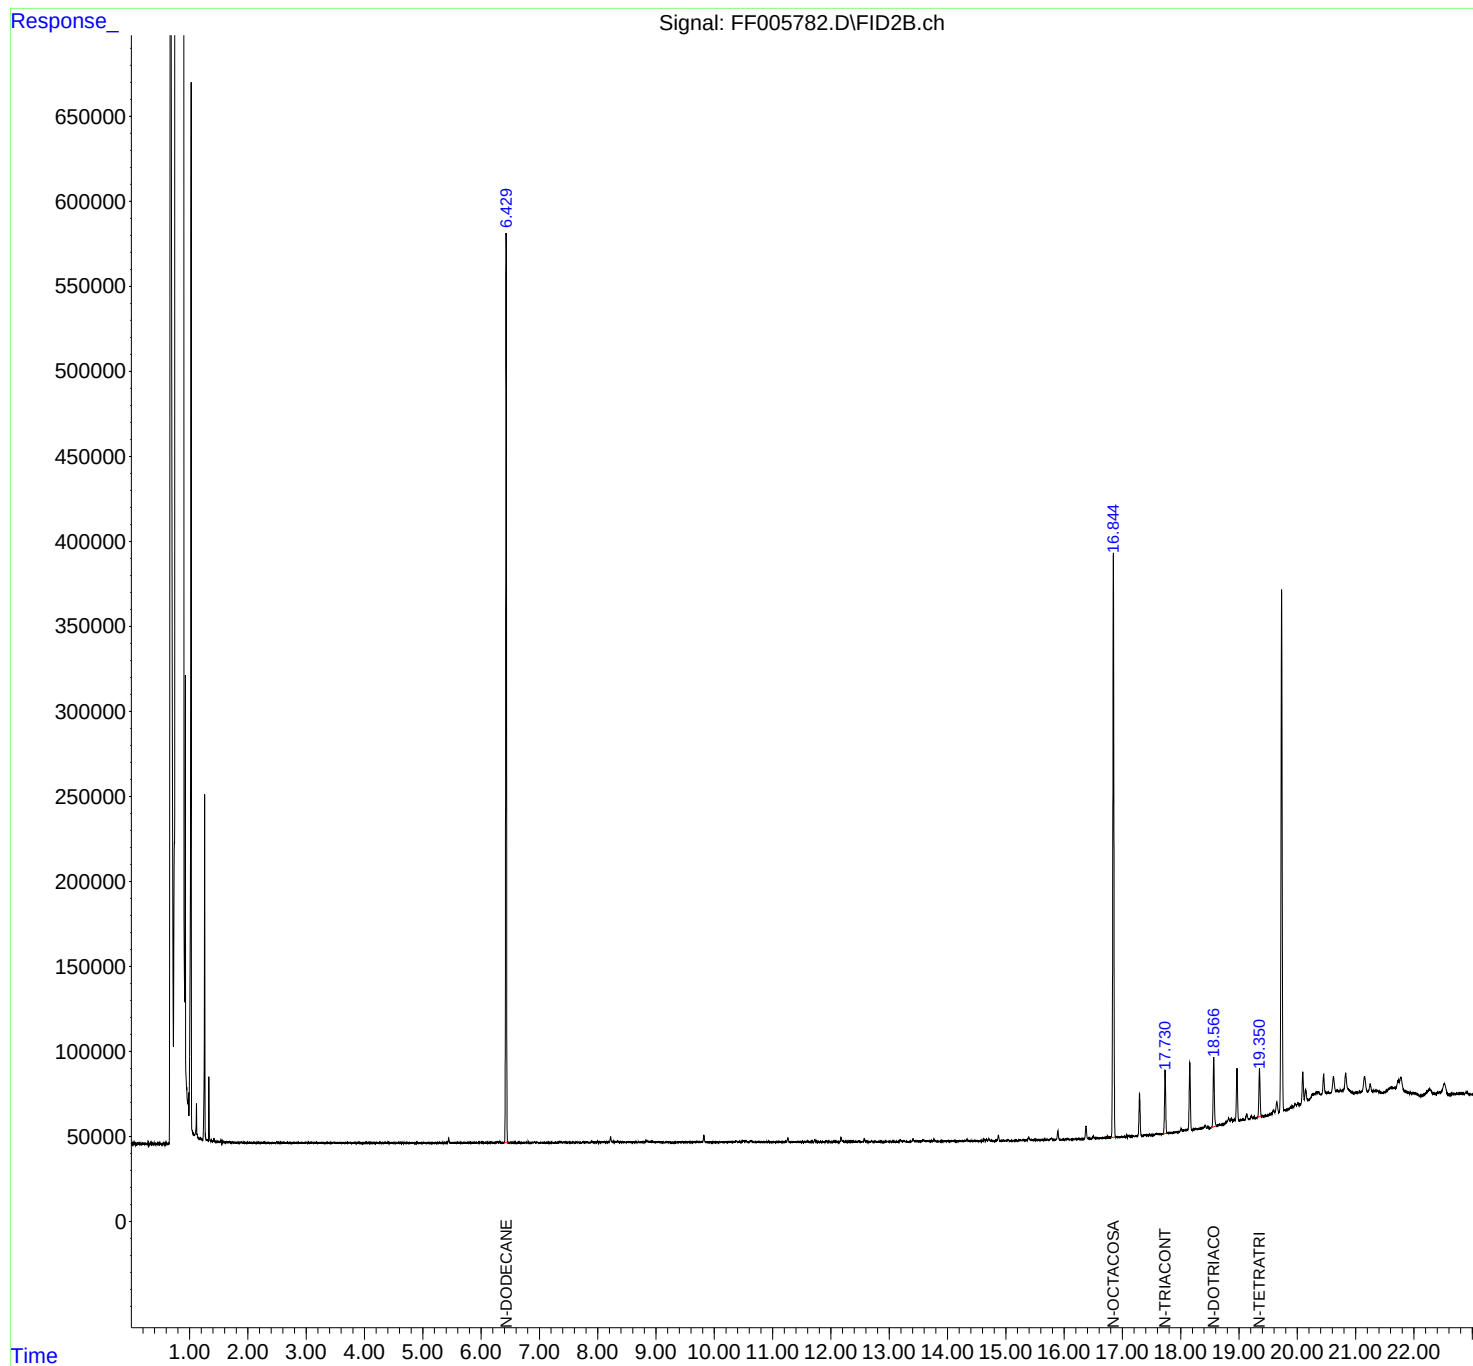


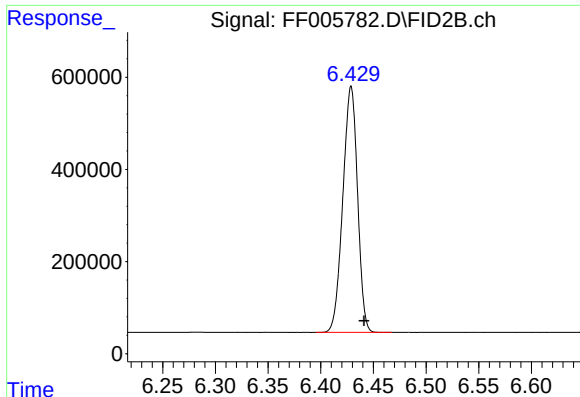

#3 N-DODECANE


R.T.: 6.429 min
Delta R.T.: -0.012 min
Response: 5192049
Conc: 32.97 ug/ml

Instrument :
FID_F
ClientSampleId :

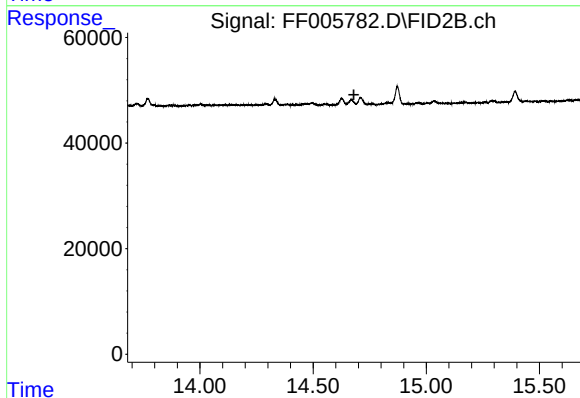


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.680 min
Response: 0
Conc: N.D.

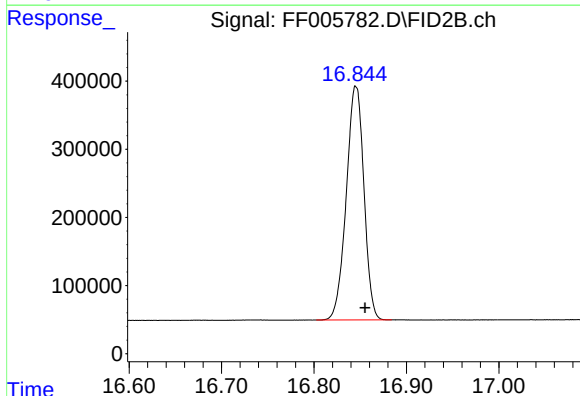


#12 N-OCTACOSANE

R.T.: 16.845 min
Delta R.T.: -0.010 min
Response: 4554026
Conc: 31.98 ug/ml

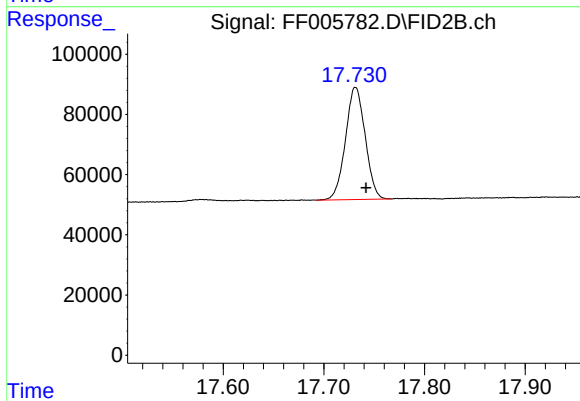

#13 N-TRIACONTANE


R.T.: 17.731 min
Delta R.T.: -0.011 min
Response: 506656
Conc: 3.65 ug/ml

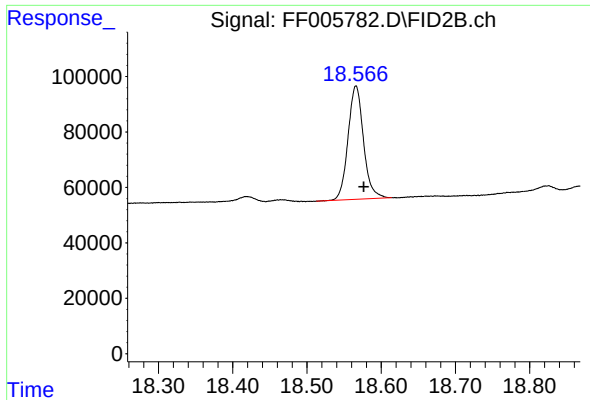

#14 N-DOTRIACONTANE

R.T.: 18.566 min
Delta R.T.: -0.010 min
Response: 590136
Conc: 4.40 ug/ml

Instrument :
FID_F
ClientSampleId :

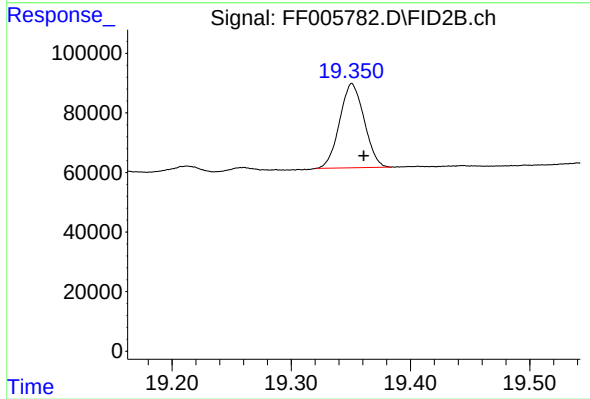

#15 N-TETRATRIACONTANE

R.T.: 19.351 min
Delta R.T.: -0.010 min
Response: 404729
Conc: 3.35 ug/ml