

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101121\
Data File : FF009110.D
Signal(s) : FID2B.ch
Acq On : 11 Oct 2021 15:07
Operator : AJ\MA
Sample : M4157-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 12 01:27:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.715	2305589	21.026 ug/ml
Target Compounds			
8) N-DOCOSANE	13.790	477667	3.778 ug/ml
13) N-TRIACONTANE	17.752	228533	2.026 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101121\
Data File : FF009110.D
Signal(s) : FID2B.ch
Acq On : 11 Oct 2021 15:07
Operator : AJ\MA
Sample : M4157-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 12 01:27:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

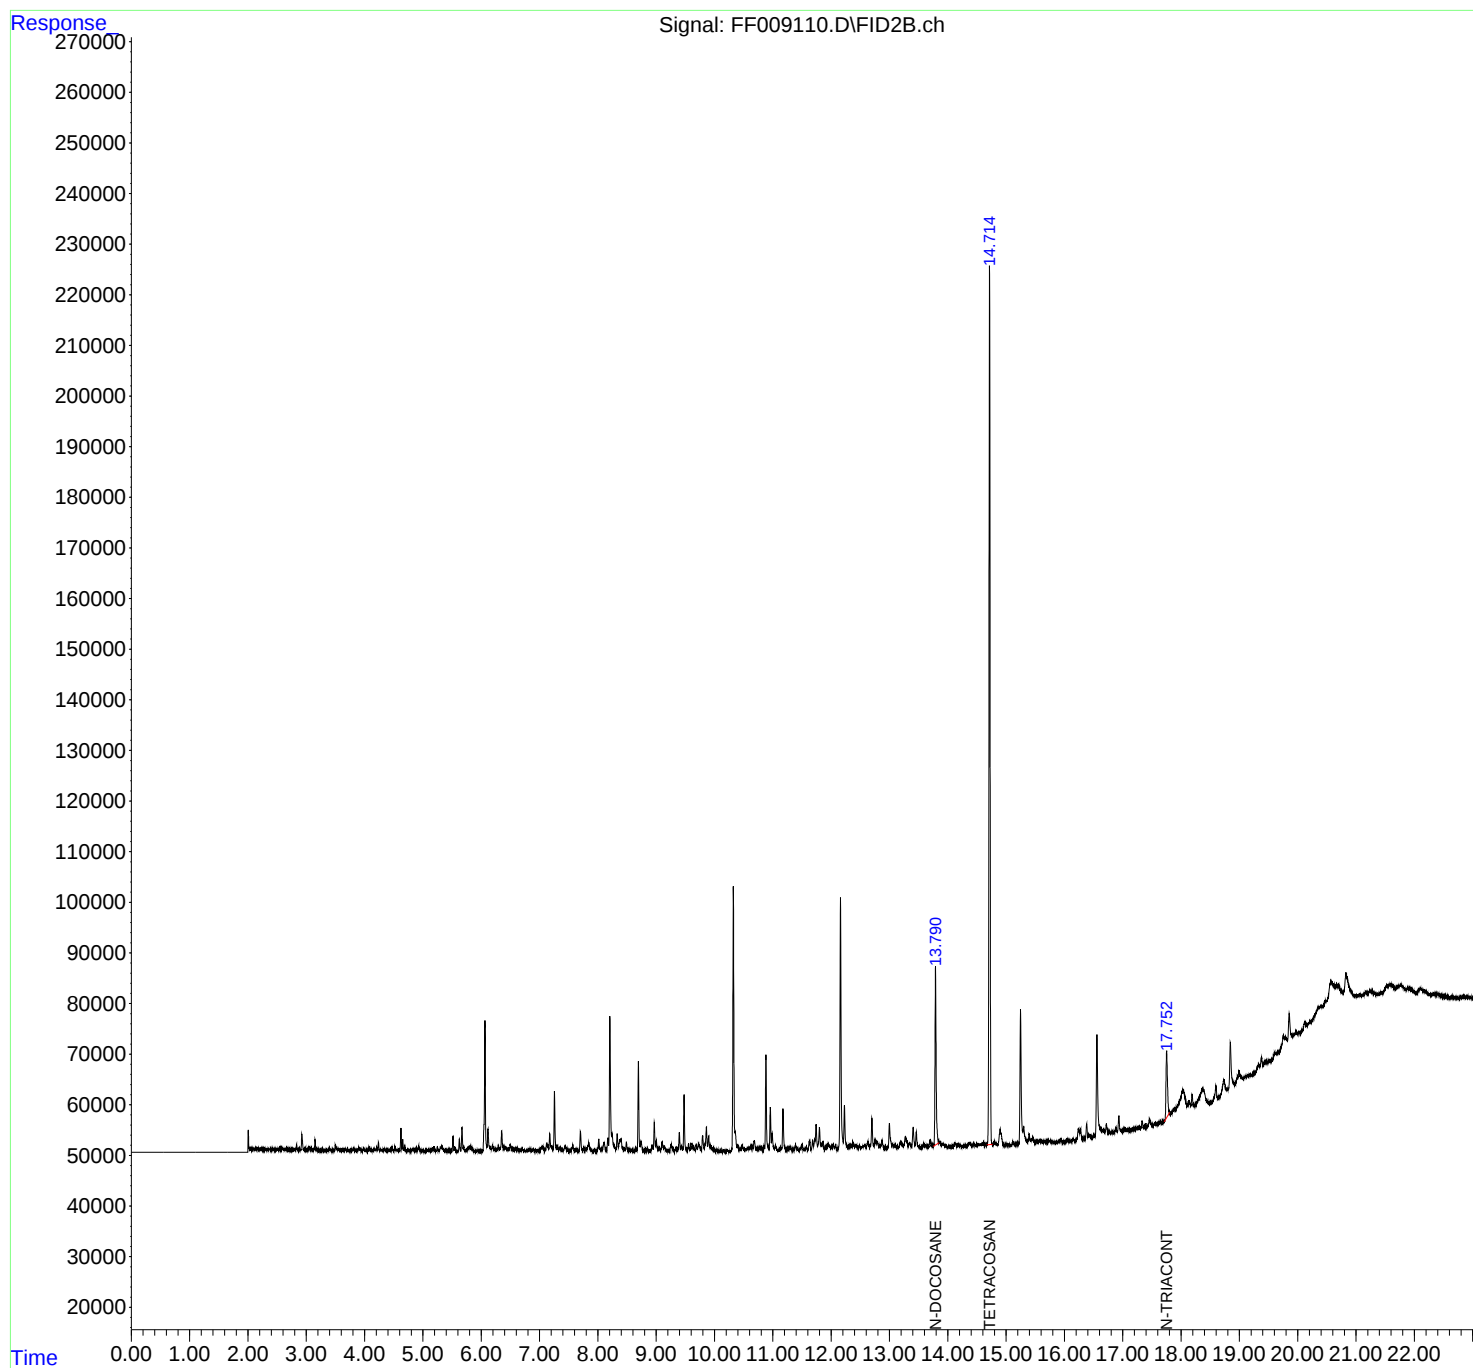


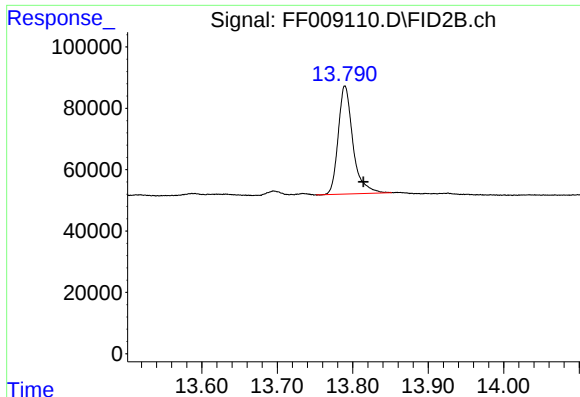

#8 N-DOCOSANE


R.T.: 13.790 min
Delta R.T.: -0.025 min
Response: 477667
Conc: 3.78 ug/ml

Instrument :
FID_F
ClientSampleId :

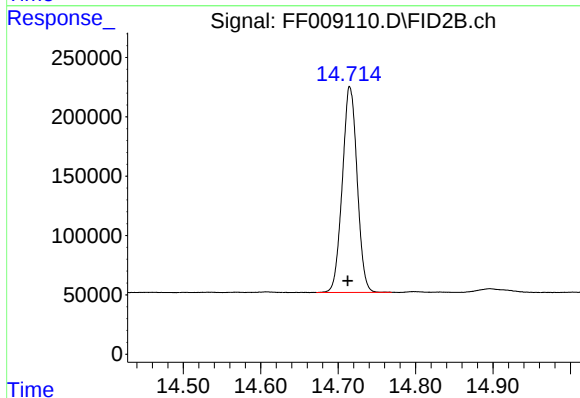

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.715 min
Delta R.T.: 0.003 min
Response: 2305589
Conc: 21.03 ug/ml

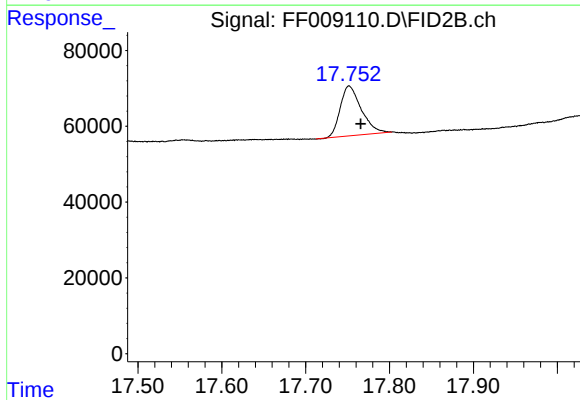

#13 N-TRIACONTANE

R.T.: 17.752 min
Delta R.T.: -0.014 min
Response: 228533
Conc: 2.03 ug/ml