

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101124\
Data File : FF014646.D
Signal(s) : FID2B.ch
Acq On : 11 Oct 2024 16:22
Operator : YP\AJ
Sample : PB164063BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB164063BL

Integration File: autoint1.e
Quant Time: Oct 14 02:08:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100324.M
Quant Title :
QLast Update : Thu Oct 03 12:23:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.884	1781478	13.622 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101124\
Data File : FF014646.D
Signal(s) : FID2B.ch
Acq On : 11 Oct 2024 16:22
Operator : YP\AJ
Sample : PB164063BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB164063BL

Integration File: autoint1.e
Quant Time: Oct 14 02:08:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100324.M
Quant Title :
QLast Update : Thu Oct 03 12:23:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

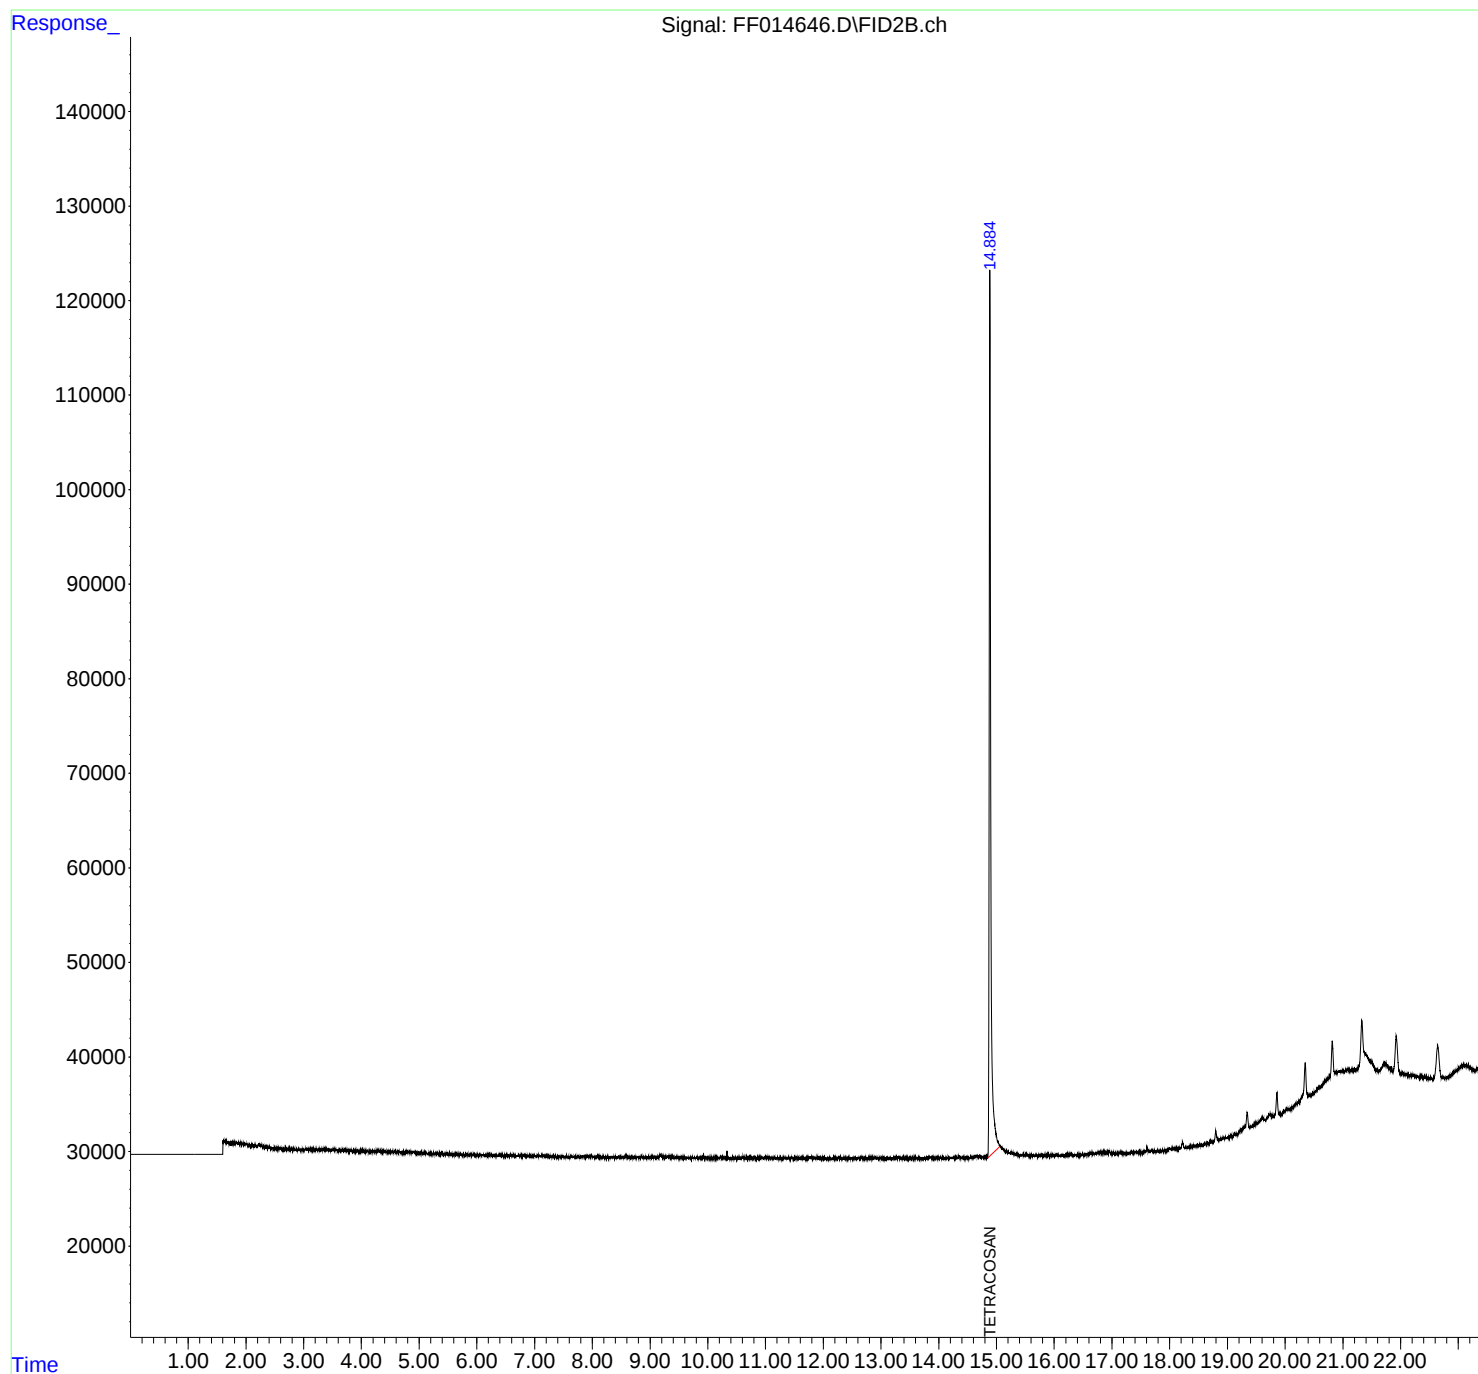

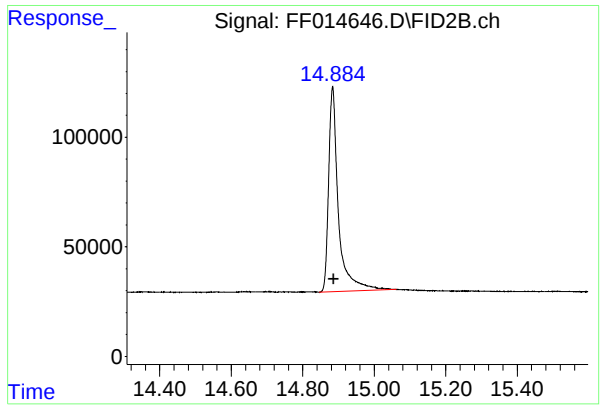

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.884 min
Delta R.T.: -0.004 min
Response: 1781478
Conc: 13.62 ug/ml

Instrument :
FID_F
ClientSampleId :
PB164063BL