

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101218\
 Data File : FB018214.D
 Signal(s) : FID2B.CH
 Acq On : 12 Oct 2018 11:27
 Operator : MJ/SJ
 Sample : BSF1012S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 12 14:45:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.112	170257	19.768 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.963	418649	27.373 ng/ml
2) t	2,2,4-Trimethylpentane	7.729	454689	30.771 ng/ml
3) t	n-Heptane	8.068	134757	9.509 ng/ml
4) t	Benzene	8.207	183658	9.859 ng/ml
6) t	Toluene	10.962	451920	29.652 ng/ml
7) t	Ethylbenzene	13.411	152472	9.610 ng/ml
8) t	m-Xylene	13.544	325687	19.574 ng/ml
9) t	O-Xylene	14.276	348875	19.567 ng/ml
10) t	1,2,4-Trimethylbenzene	16.559	408159	20.064 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101218\
Data File : FB018214.D
Signal(s) : FID2B.CH
Acq On : 12 Oct 2018 11:27
Operator : MJ/SJ
Sample : BSF1012S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 12 14:45:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

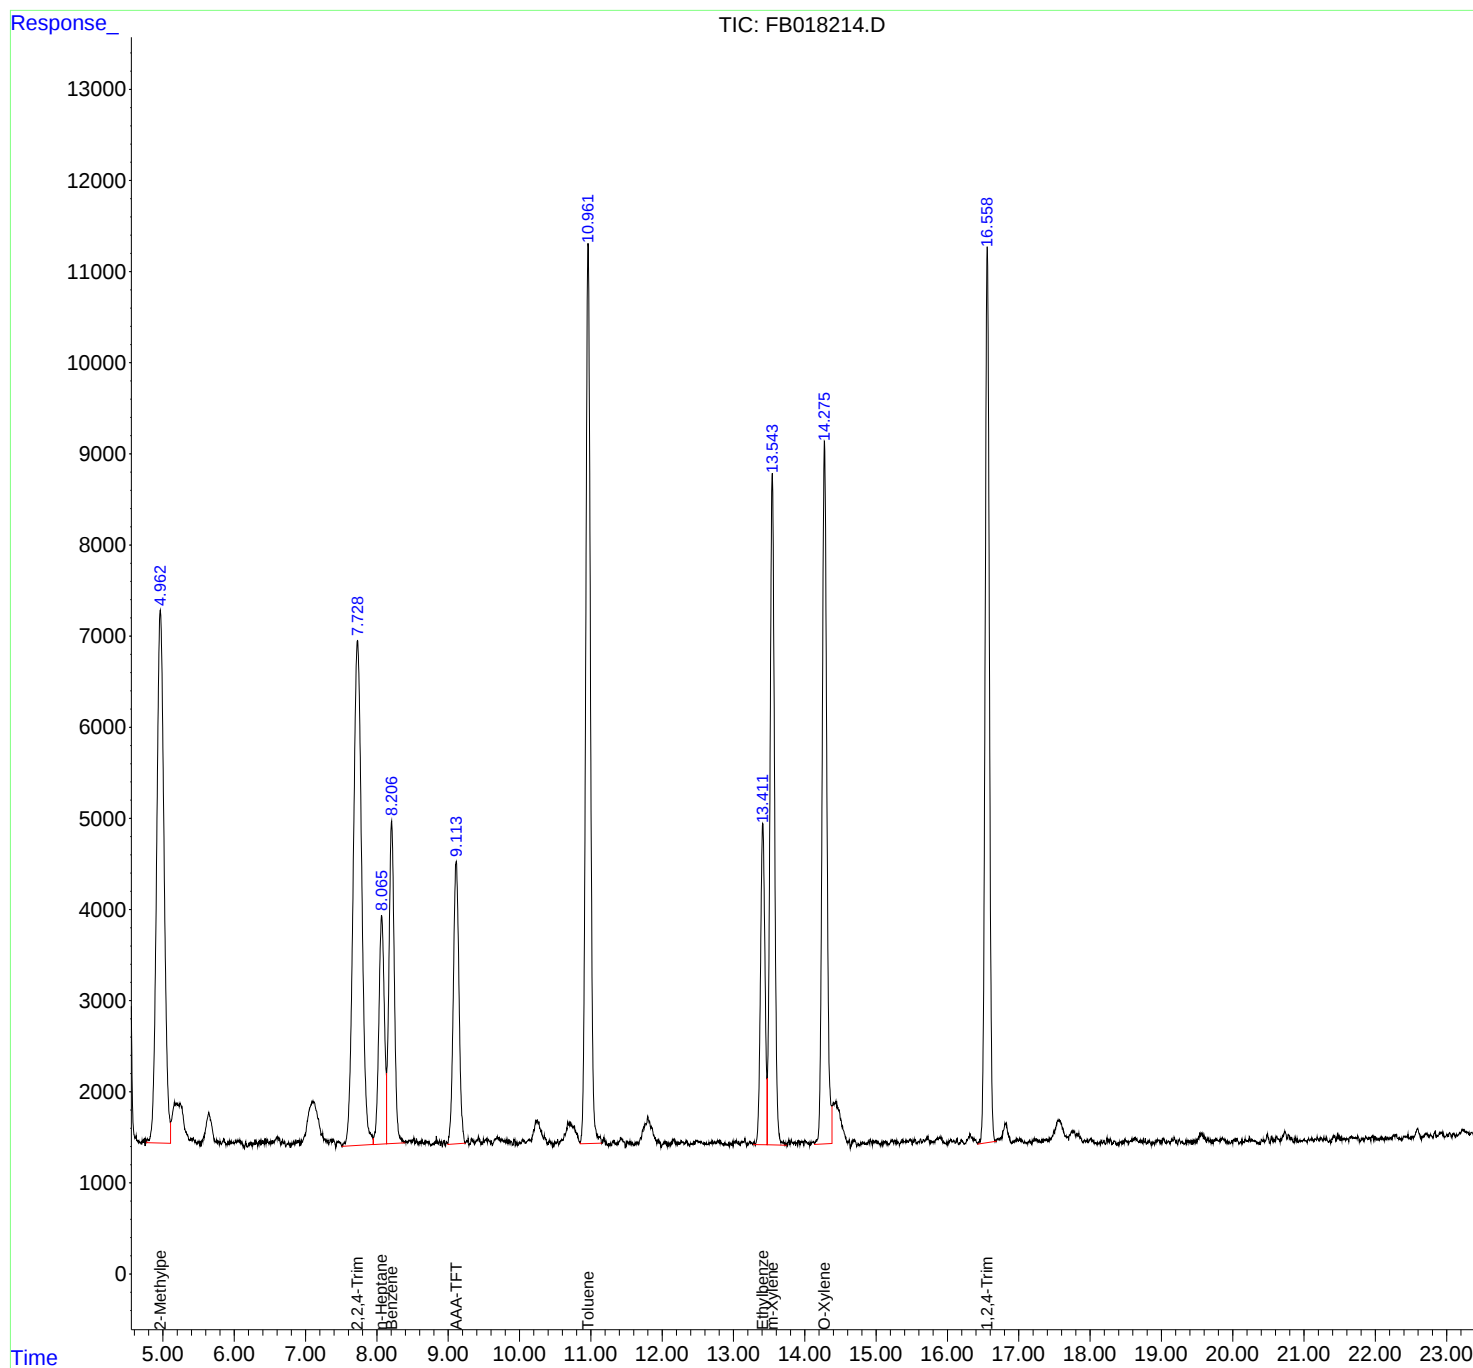

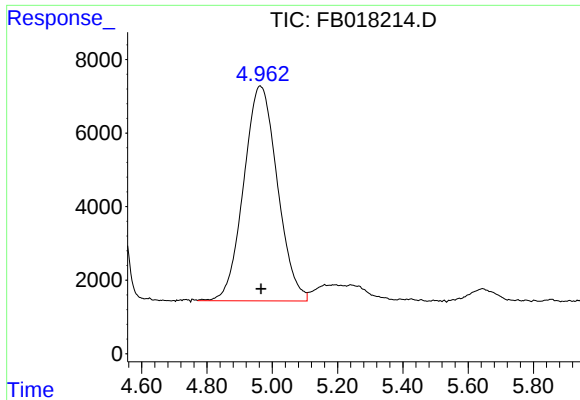


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 418649
Conc: 27.37 ng/ml

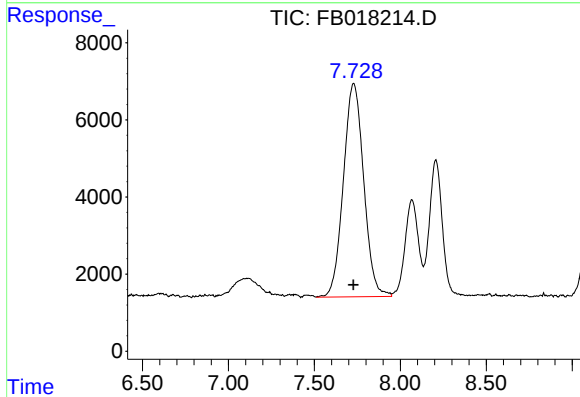


#2 2,2,4-Trimethylpentane

R.T.: 7.729 min
Delta R.T.: 0.000 min
Response: 454689
Conc: 30.77 ng/ml

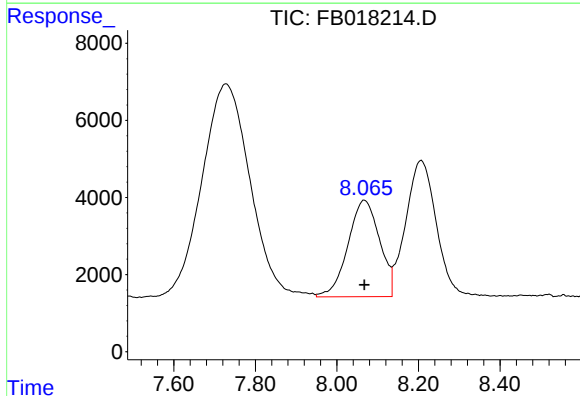


#3 n-Heptane

R.T.: 8.068 min
Delta R.T.: 0.000 min
Response: 134757
Conc: 9.51 ng/ml

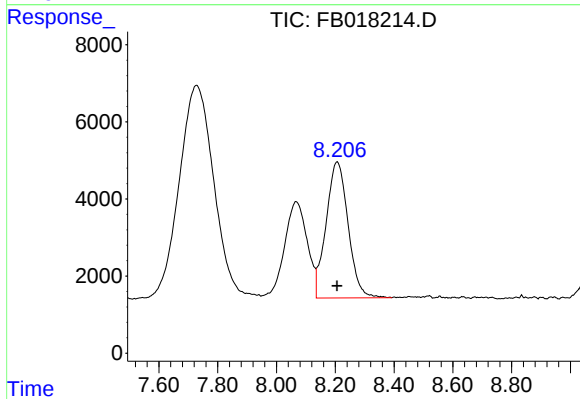


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 183658
Conc: 9.86 ng/ml

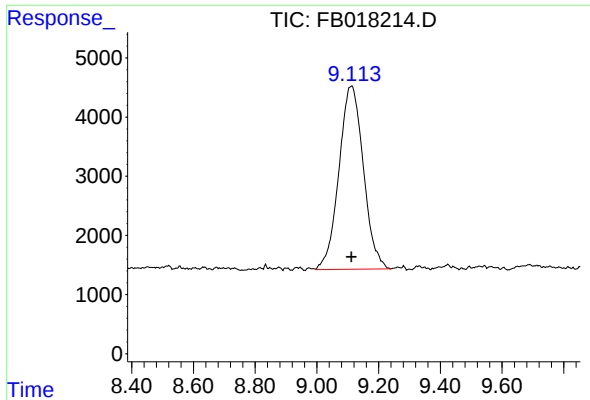


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 170257
Conc: 19.77 ng/ml

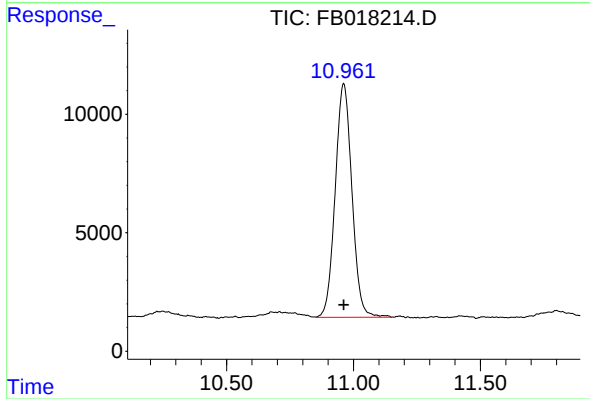


#6 Toluene

R.T.: 10.962 min
Delta R.T.: 0.000 min
Response: 451920
Conc: 29.65 ng/ml

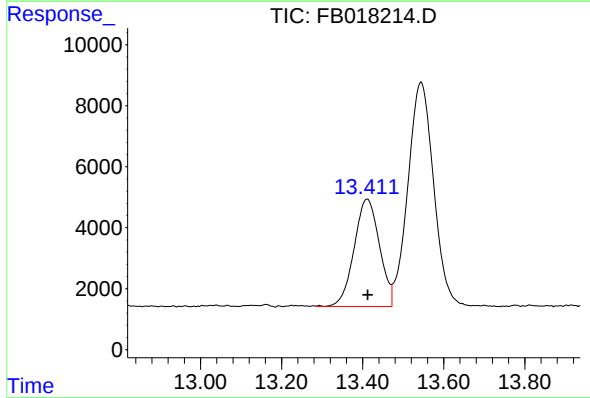


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 152472
Conc: 9.61 ng/ml

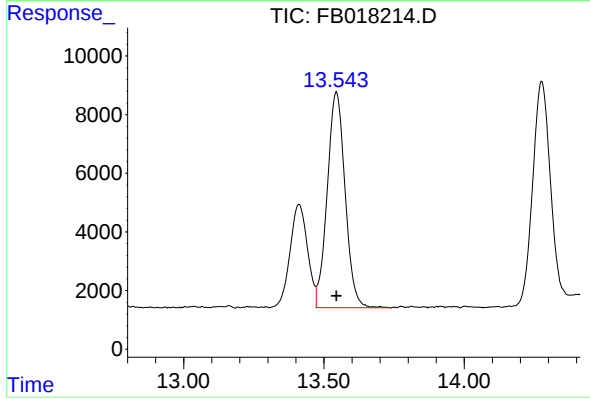


#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 325687
Conc: 19.57 ng/ml

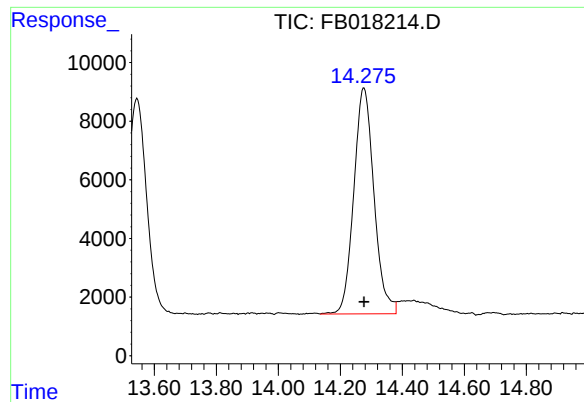

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.000 min
Response: 348875
Conc: 19.57 ng/ml

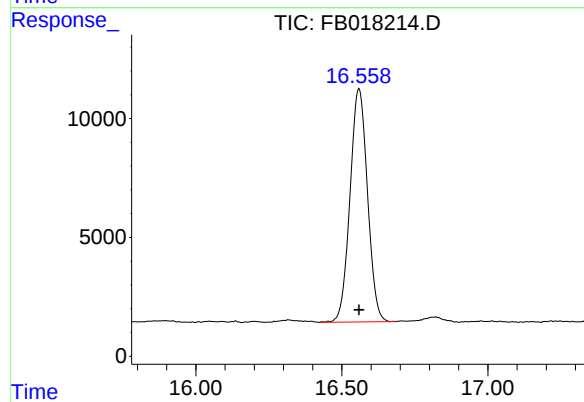

#10 1,2,4-Trimethylbenzene

R.T.: 16.559 min
Delta R.T.: 0.000 min
Response: 408159
Conc: 20.06 ng/ml