

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101421\
Data File : FF009117.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2021 11:04
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 23:50:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
12)	N-OCTACOSANE	16.880	102427	0.875 ug/ml
13)	N-TRIACONTANE	17.764	206114	1.827 ug/ml
14)	N-DOTRIACONTANE	18.595	123476	1.169 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101421\
Data File : FF009117.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2021 11:04
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 23:50:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

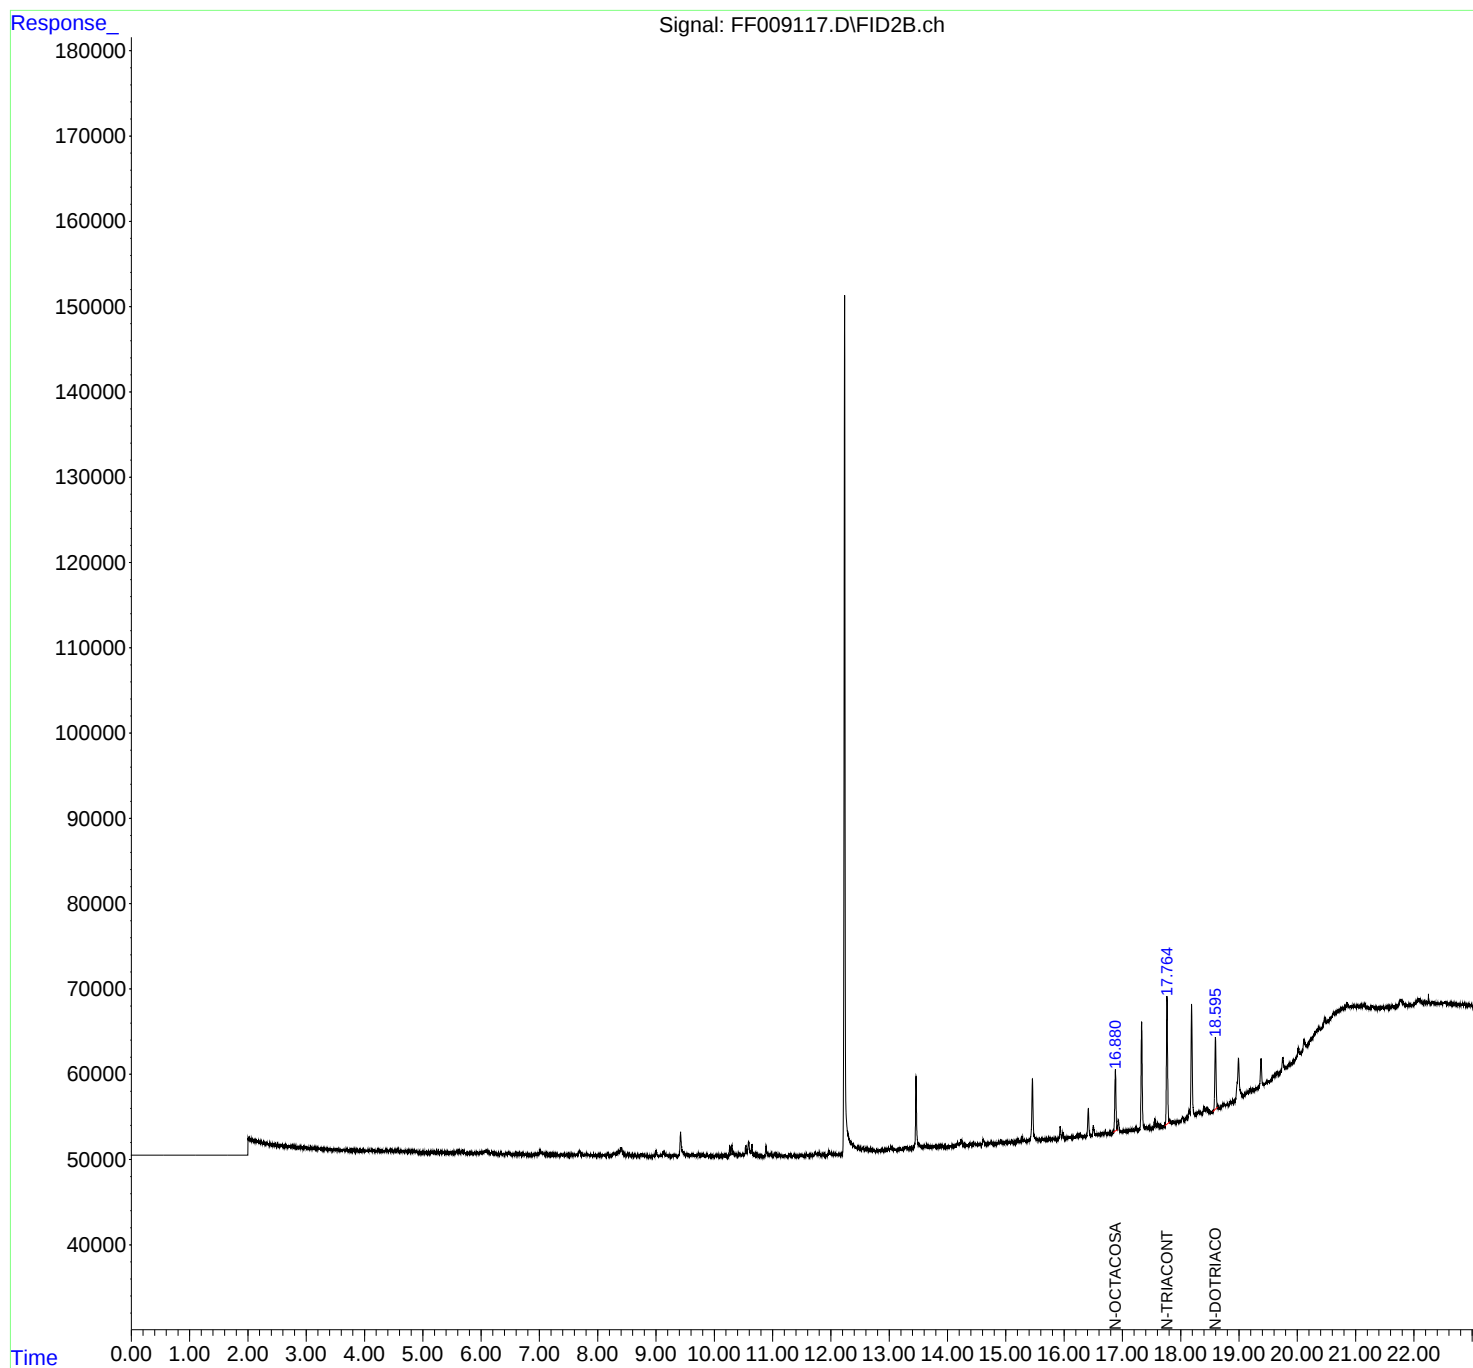


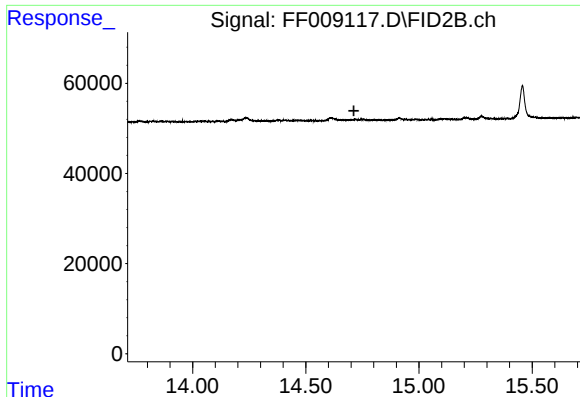

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.712 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

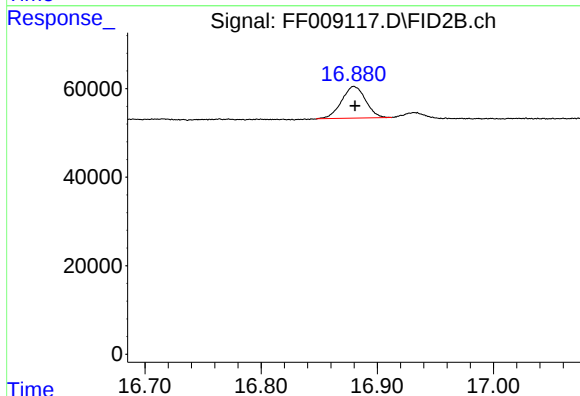


#12 N-OCTACOSANE

R.T.: 16.880 min
Delta R.T.: 0.000 min
Response: 102427
Conc: 0.87 ug/ml

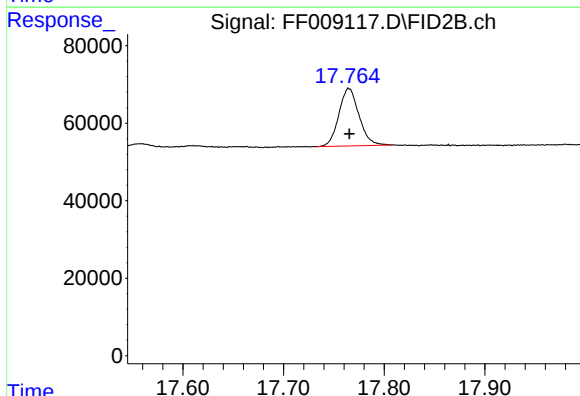

#13 N-TRIACONTANE

R.T.: 17.764 min
Delta R.T.: -0.001 min
Response: 206114
Conc: 1.83 ug/ml

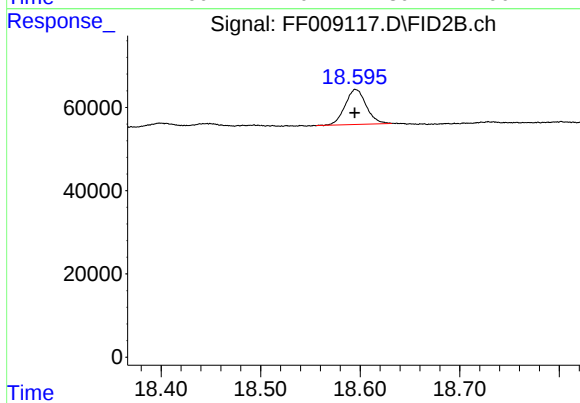

#14 N-DOTRIACONTANE

R.T.: 18.595 min
Delta R.T.: 0.000 min
Response: 123476
Conc: 1.17 ug/ml