

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101421\
Data File : FF009118.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2021 11:35
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 23:50:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	2504468	22.839 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.763	155877	1.382 ug/ml
14) N-DOTRIACONTANE	18.596	119411	1.131 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101421\
Data File : FF009118.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2021 11:35
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 23:50:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

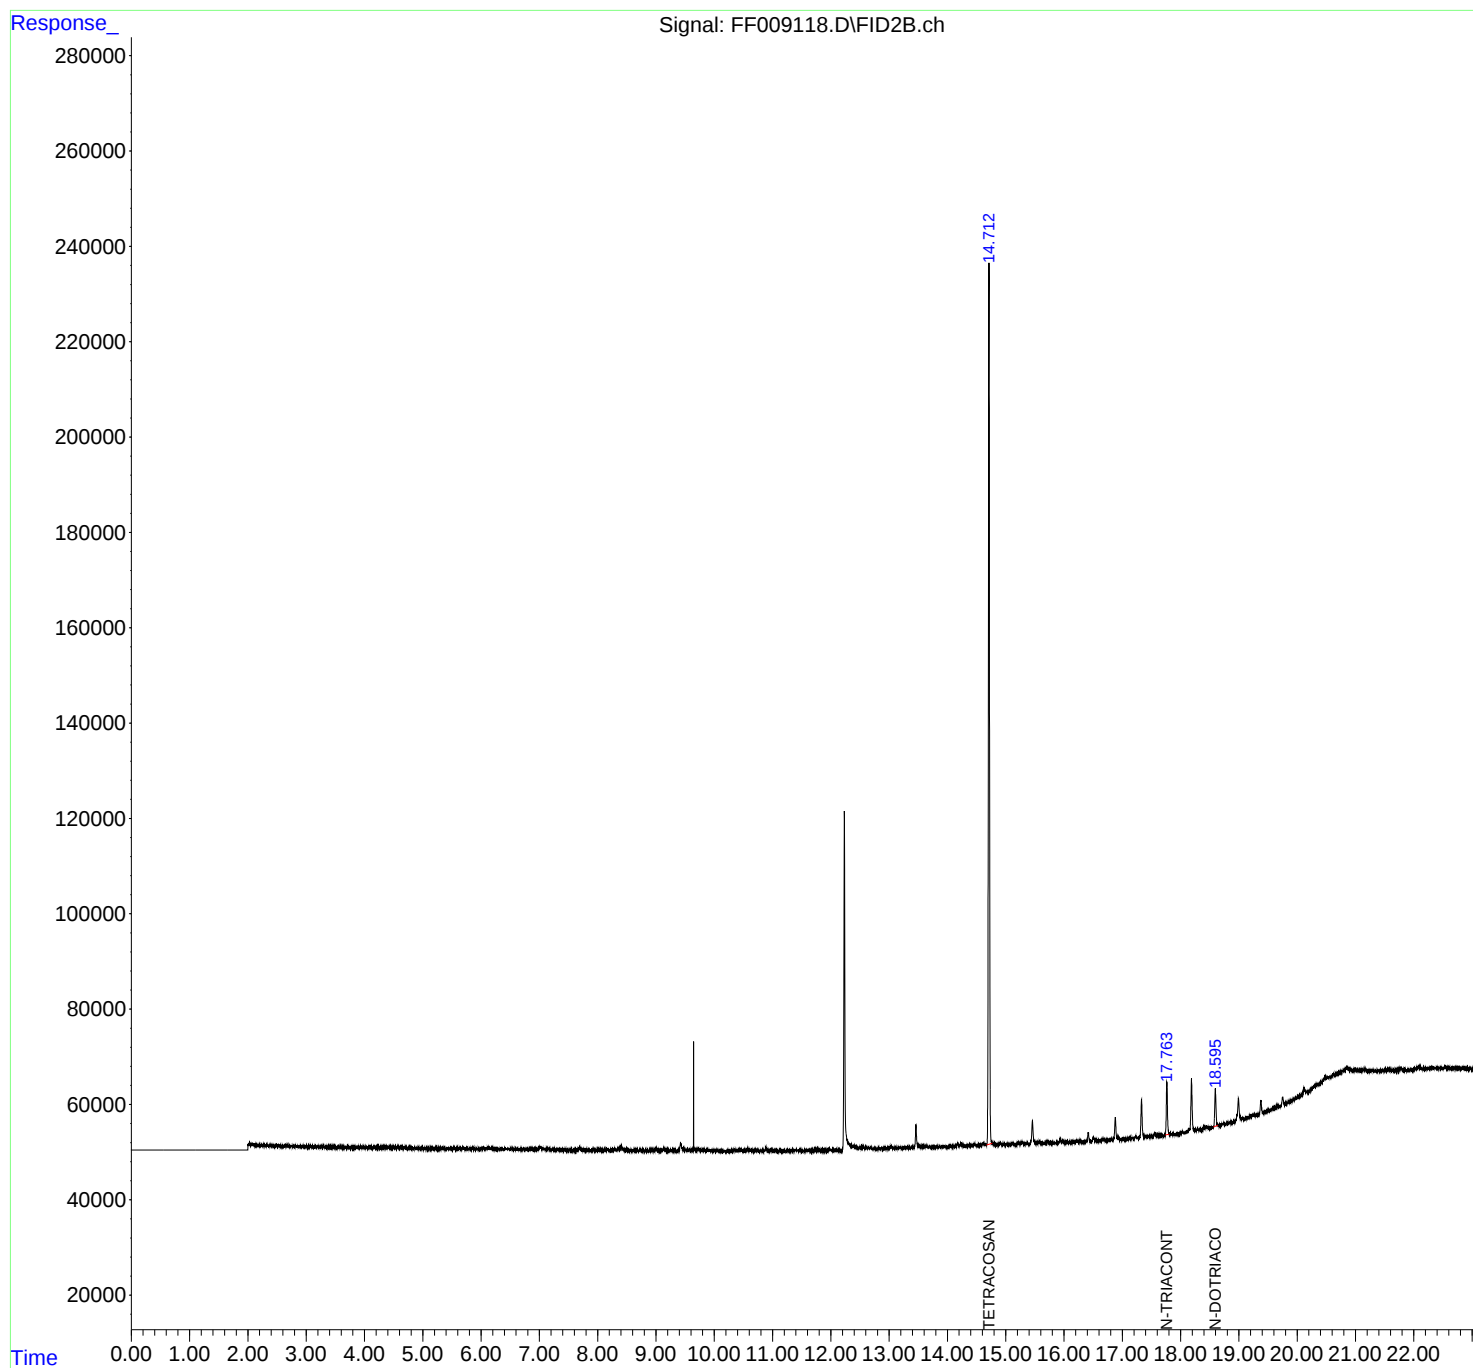


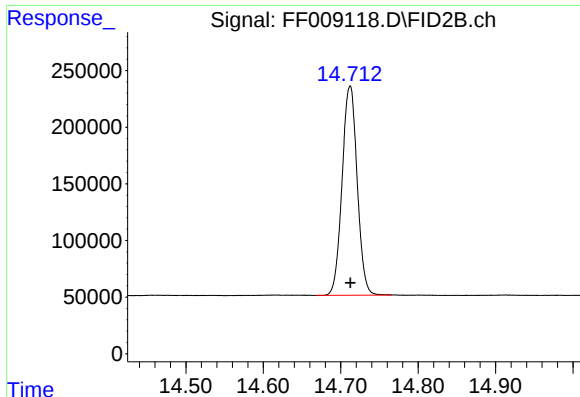

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.712 min
Delta R.T.: 0.000 min
Response: 2504468
Conc: 22.84 ug/ml

Instrument :
FID_F
ClientSampleId :

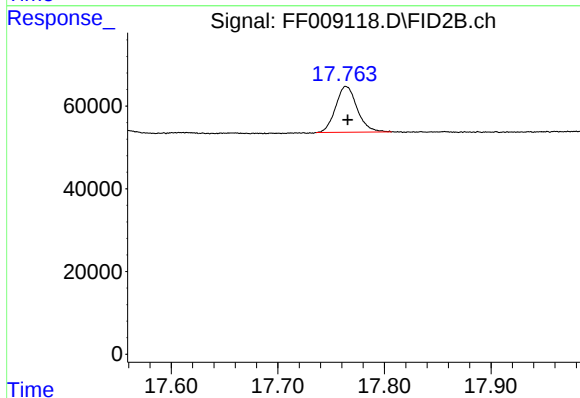

#13 N-TRIACONTANE

R.T.: 17.763 min
Delta R.T.: -0.002 min
Response: 155877
Conc: 1.38 ug/ml

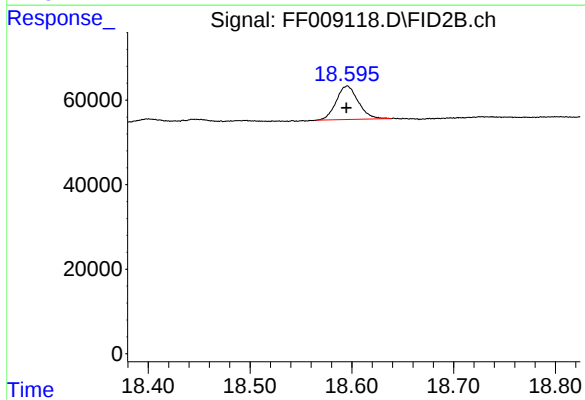

#14 N-DOTRIACONTANE

R.T.: 18.596 min
Delta R.T.: 0.001 min
Response: 119411
Conc: 1.13 ug/ml