

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101421\
Data File : FF009120.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2021 12:36
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 23:51:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.483	2725608	21.455 ug/ml
12) N-OCTACOSANE	16.880	2811214	24.014 ug/ml
13) N-TRIACONTANE	17.764	119910	1.063 ug/ml
14) N-DOTRIACONTANE	18.593	124310	1.177 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101421\
Data File : FF009120.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2021 12:36
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 23:51:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

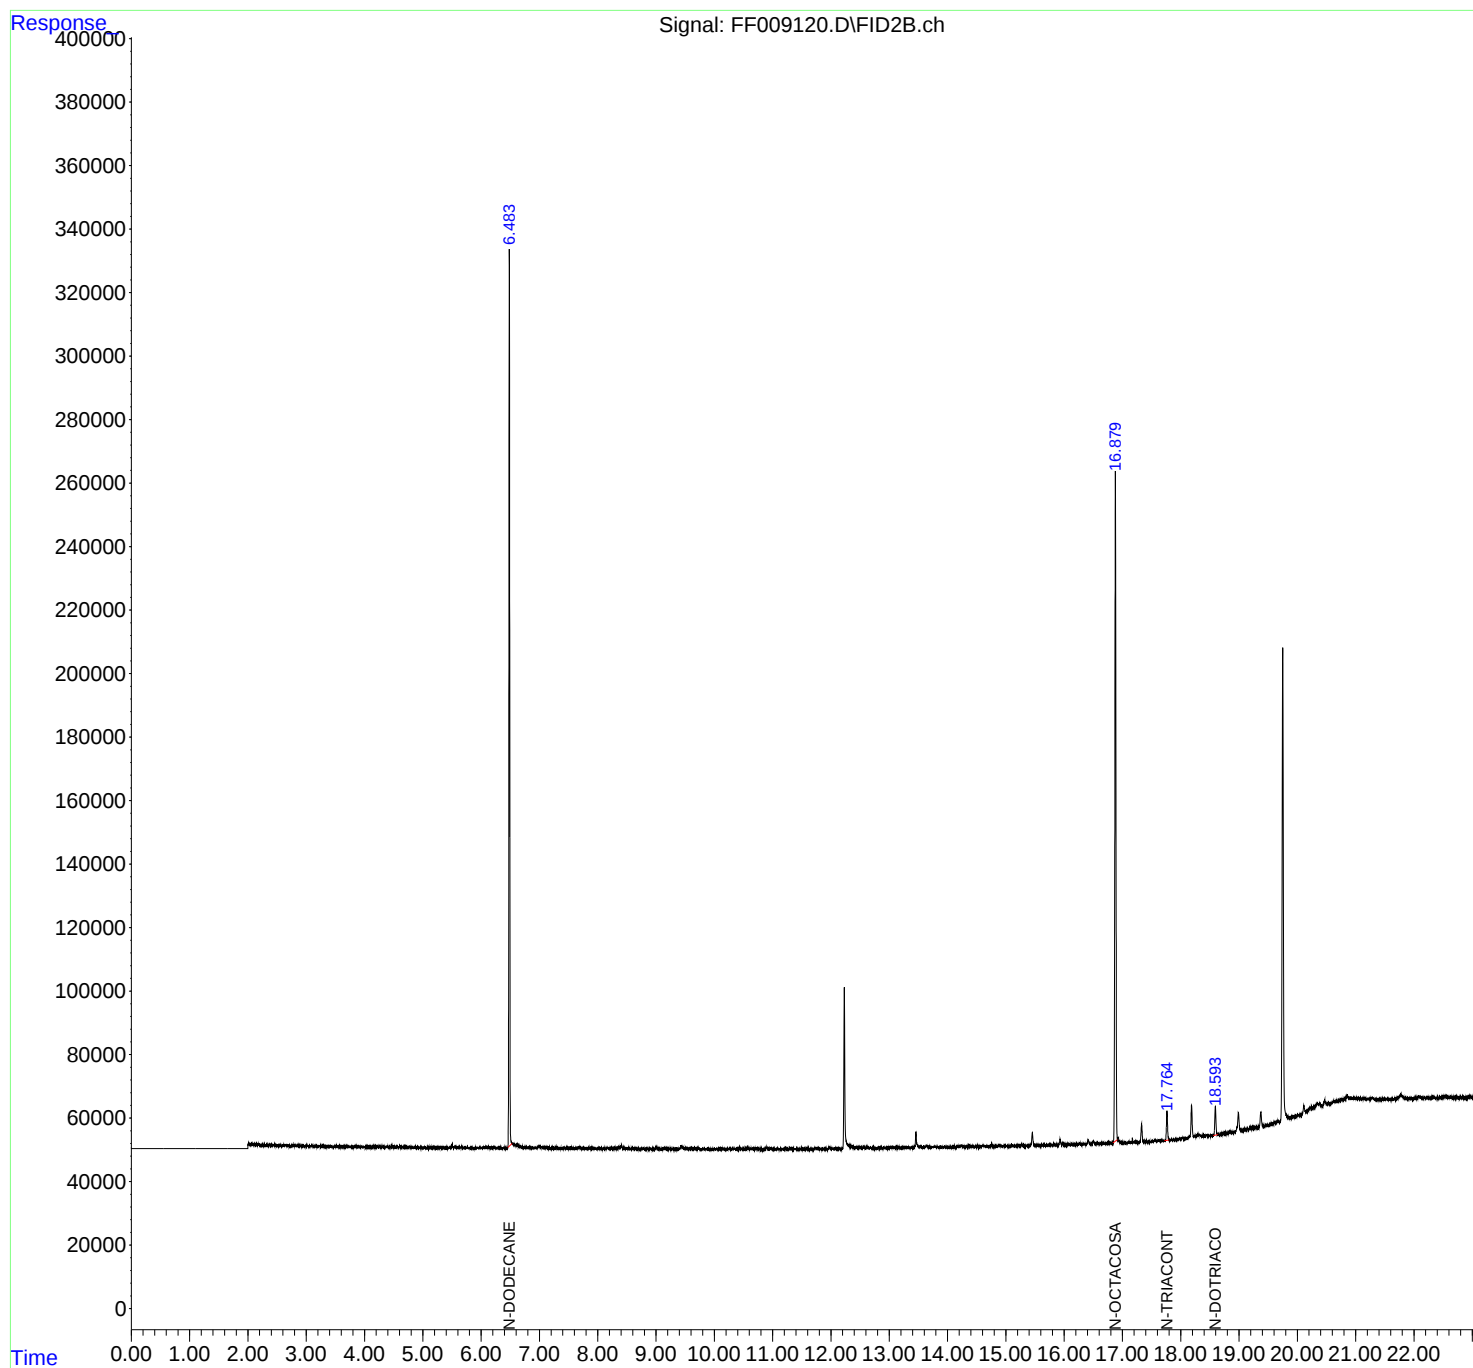


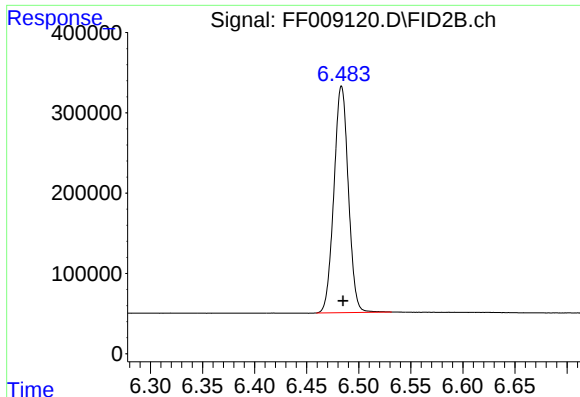

#3 N-DODECANE


R.T.: 6.483 min
Delta R.T.: -0.001 min
Response: 2725608
Conc: 21.45 ug/ml

Instrument :
FID_F
ClientSampleId :

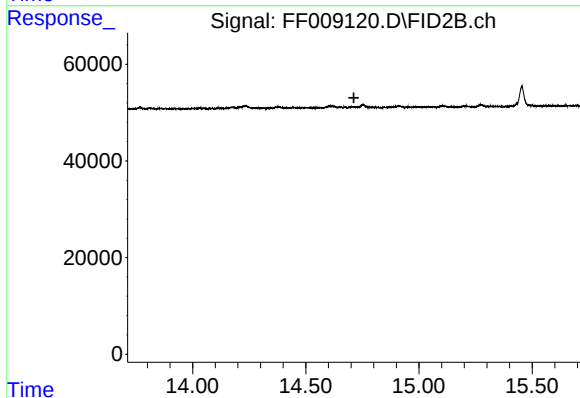


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.

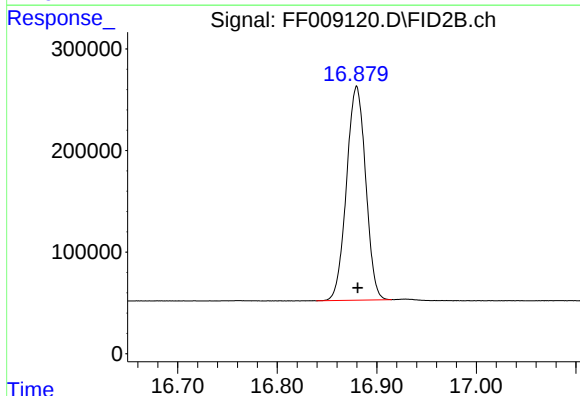


#12 N-OCTACOSANE

R.T.: 16.880 min
Delta R.T.: 0.000 min
Response: 2811214
Conc: 24.01 ug/ml

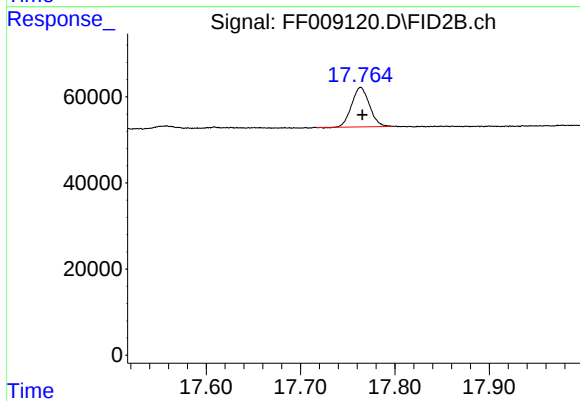

#13 N-TRIACONTANE

R.T.: 17.764 min
Delta R.T.: -0.002 min
Response: 119910
Conc: 1.06 ug/ml

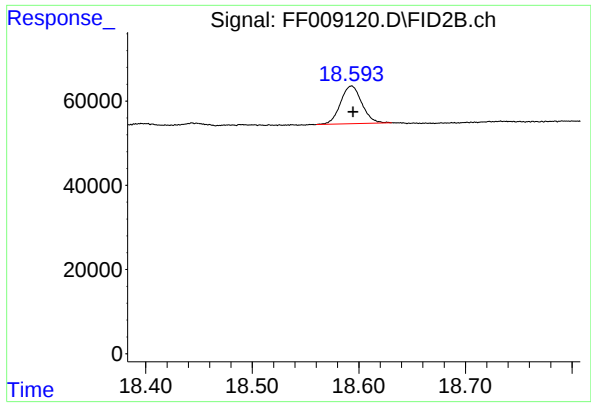

#14 N-DOTRIACONTANE

R.T.: 18.593 min
Delta R.T.: -0.001 min
Response: 124310
Conc: 1.18 ug/ml

Instrument :

FID_F

ClientSampleId :