

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101421\
 Data File : FF009126.D
 Signal(s) : FID2B.ch
 Acq On : 14 Oct 2021 16:21
 Operator : AJ\MA
 Sample : M4068-07
 Misc : LOD 1 PPB
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 14 23:52:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
 Quant Title :
 QLast Update : Fri Oct 08 02:25:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	2162668	19.722 ug/ml
Target Compounds			
1) N-OCTANE	2.370	117297	0.938 ug/ml
2) N-DECANE	4.466	122875	0.969 ug/ml
3) N-DODECANE	6.482	103601	0.815 ug/ml
5) N-HEXADECANE	9.876	114130	0.899 ug/ml
6) N-OCTADECANE	11.312	119074	0.924 ug/ml
7) N-EICOSANE	12.617	130401	1.013 ug/ml
8) N-DOCOSANE	13.813	131863	1.043 ug/ml
10) N-TETRACOSANE	14.913	127427	1.018 ug/ml
11) N-HEXACOSANE	15.934	115763	0.956 ug/ml
12) N-OCTACOSANE	16.882	120580	1.030 ug/ml
13) N-TRIACONTANE	17.766	141341	1.253 ug/ml
14) N-DOTRIACONTANE	18.596	142488	1.349 ug/ml
15) N-TETRATRIACONTANE	19.377	98110	1.004 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101421\
Data File : FF009126.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2021 16:21
Operator : AJ\MA
Sample : M4068-07
Misc : LOD 1 PPB
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 23:52:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

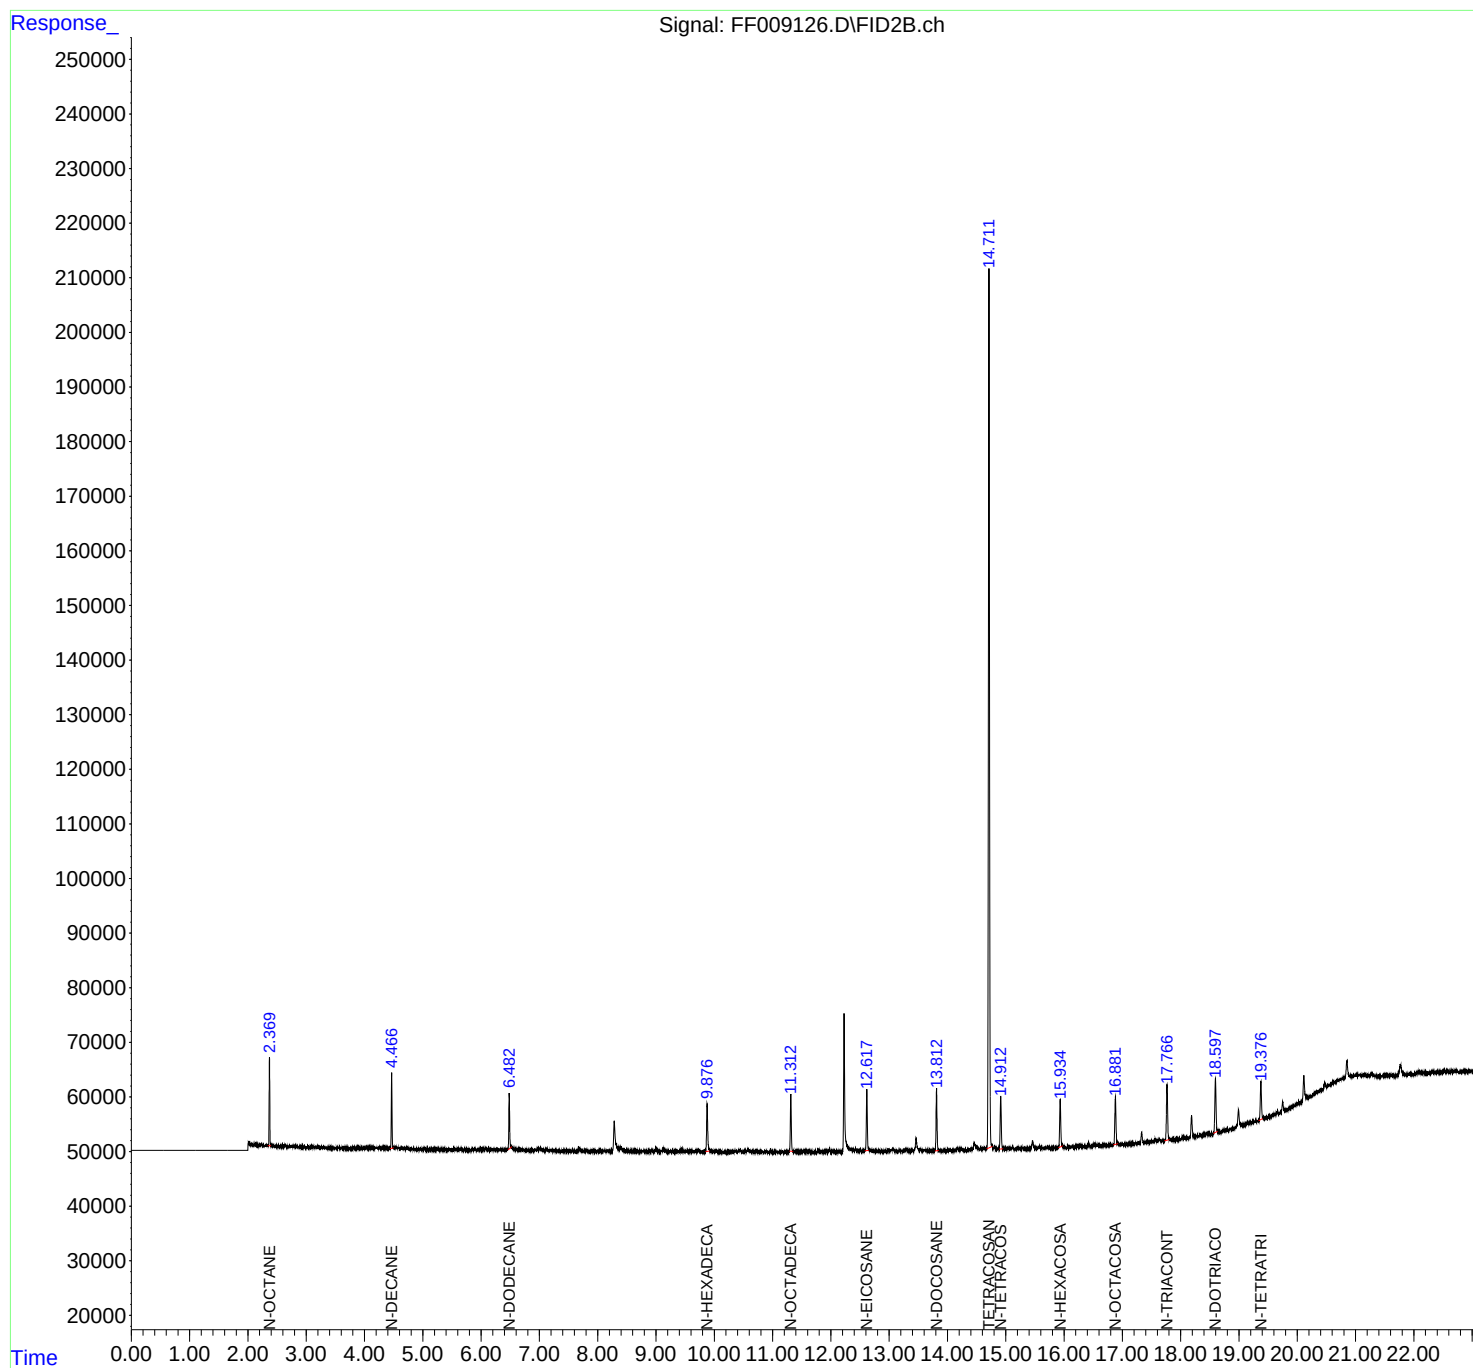


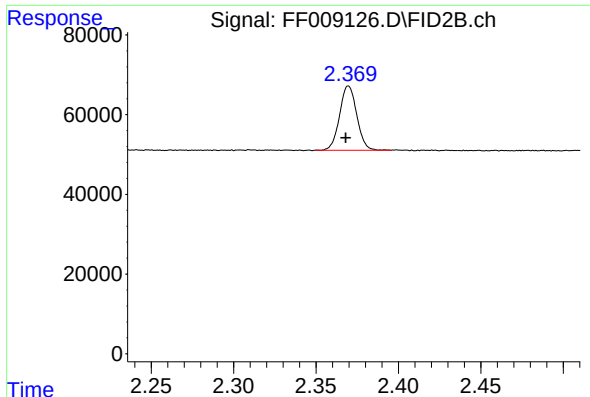

#1 N-OCTANE


R.T.: 2.370 min
Delta R.T.: 0.002 min
Response: 117297
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :

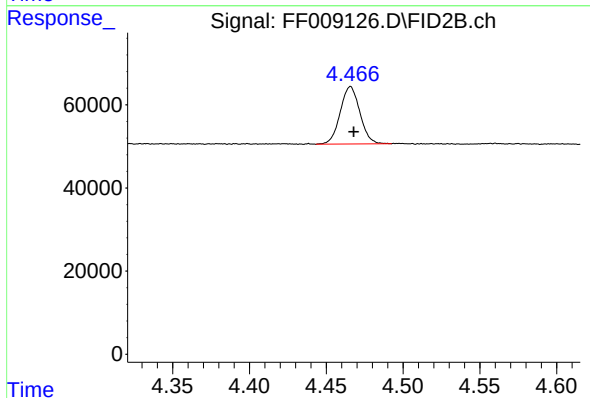


#2 N-DECANE

R.T.: 4.466 min
Delta R.T.: -0.002 min
Response: 122875
Conc: 0.97 ug/ml

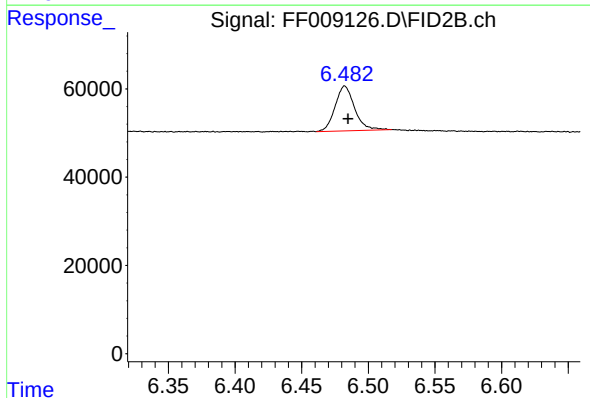


#3 N-DODECANE

R.T.: 6.482 min
Delta R.T.: -0.003 min
Response: 103601
Conc: 0.82 ug/ml

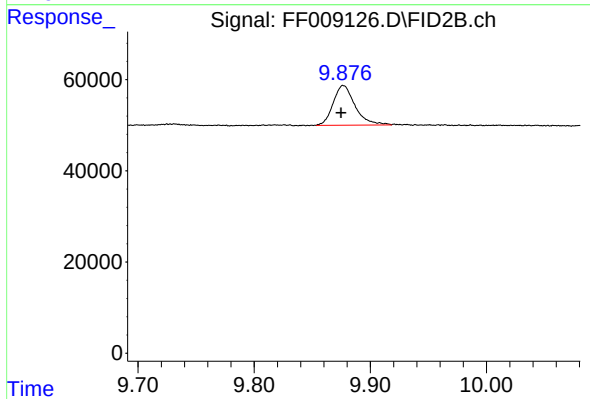

#5 N-HEXADECANE


R.T.: 9.876 min
Delta R.T.: 0.001 min
Response: 114130
Conc: 0.90 ug/ml

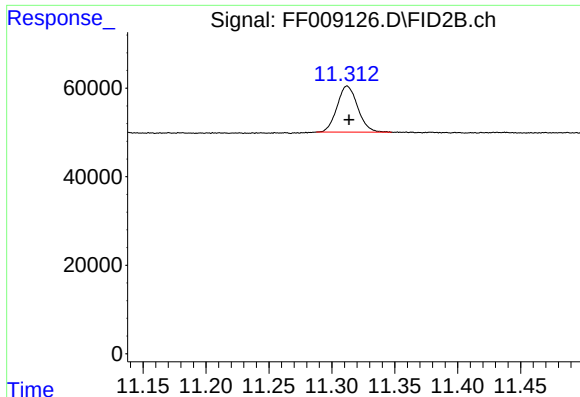

#6 N-OCTADECANE


R.T.: 11.312 min
Delta R.T.: -0.001 min
Response: 119074
Conc: 0.92 ug/ml

Instrument :
FID_F
ClientSampleId :

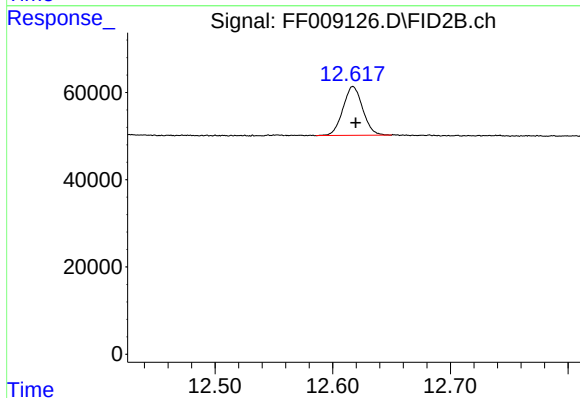


#7 N-EICOSANE

R.T.: 12.617 min
Delta R.T.: -0.002 min
Response: 130401
Conc: 1.01 ug/ml

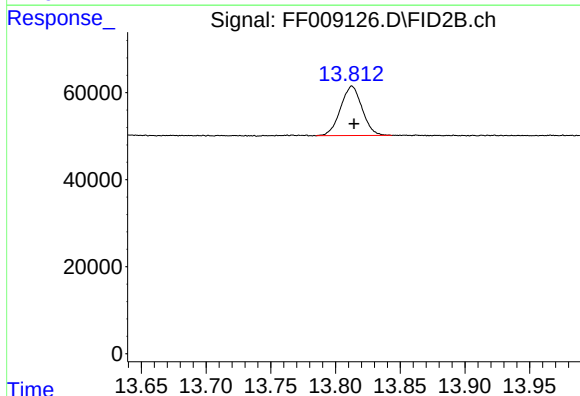


#8 N-DOCOSANE

R.T.: 13.813 min
Delta R.T.: -0.002 min
Response: 131863
Conc: 1.04 ug/ml

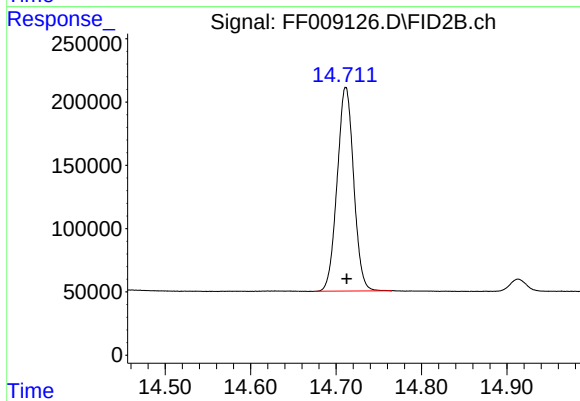

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.711 min
Delta R.T.: -0.001 min
Response: 2162668
Conc: 19.72 ug/ml

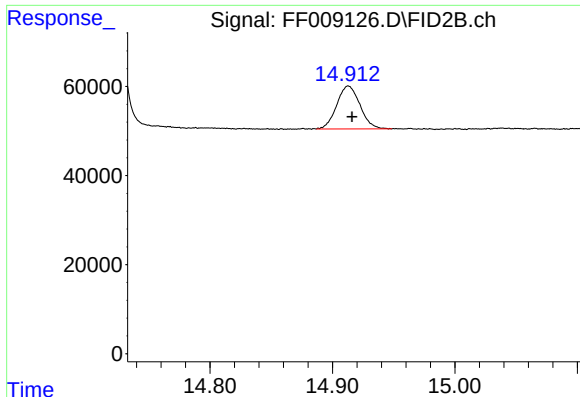

#10 N-TETRACOSANE


R.T.: 14.913 min
Delta R.T.: -0.003 min
Response: 127427
Conc: 1.02 ug/ml

Instrument :
FID_F
ClientSampleId :

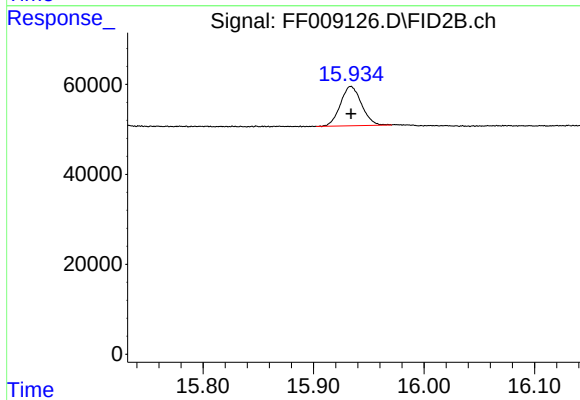


#11 N-HEXACOSANE

R.T.: 15.934 min
Delta R.T.: 0.000 min
Response: 115763
Conc: 0.96 ug/ml

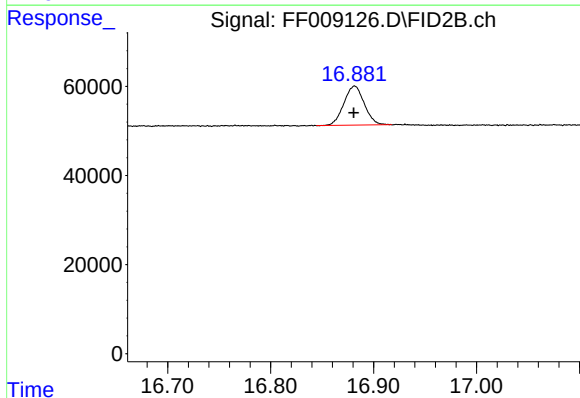


#12 N-OCTACOSANE

R.T.: 16.882 min
Delta R.T.: 0.000 min
Response: 120580
Conc: 1.03 ug/ml

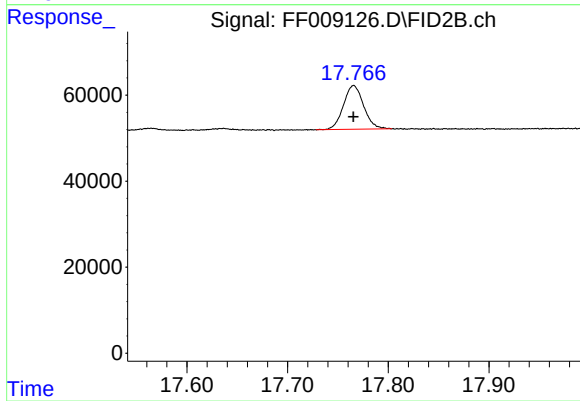

#13 N-TRIACONTANE


R.T.: 17.766 min
Delta R.T.: 0.000 min
Response: 141341
Conc: 1.25 ug/ml

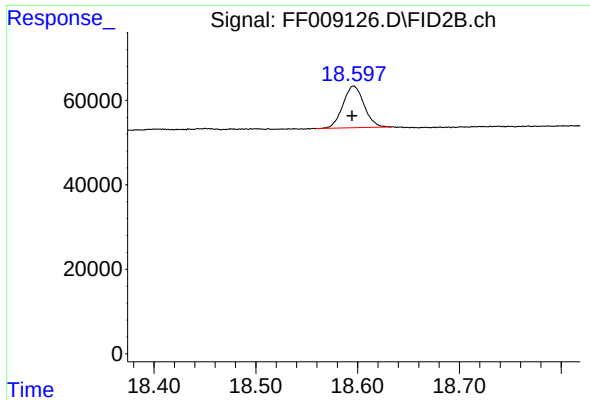

#14 N-DOTRIACONTANE

R.T.: 18.596 min
Delta R.T.: 0.002 min
Response: 142488
Conc: 1.35 ug/ml

Instrument :
FID_F
ClientSampleId :

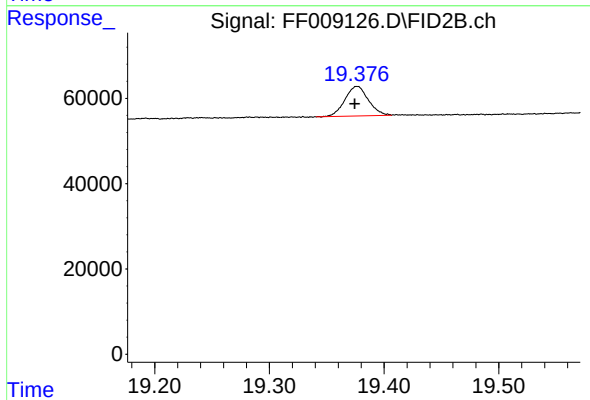

#15 N-TETRATRIACONTANE

R.T.: 19.377 min
Delta R.T.: 0.002 min
Response: 98110
Conc: 1.00 ug/ml