

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101424AL\
Data File : FF014673.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2024 20:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 15 02:11:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100224.M
Quant Title : GC Extractables
QLast Update : Wed Oct 02 12:50:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.797	387548	2.529 ug/ml
20) T	n-Hexatriacontane (C36)	20.346f	1056518	10.205 ug/ml
22) T	n-Tetracontane (C40)	21.926f	1851676	23.658 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101424AL\
Data File : FF014673.D
Signal(s) : FID2B.ch
Acq On : 14 Oct 2024 20:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 15 02:11:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100224.M
Quant Title : GC Extractables
QLast Update : Wed Oct 02 12:50:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

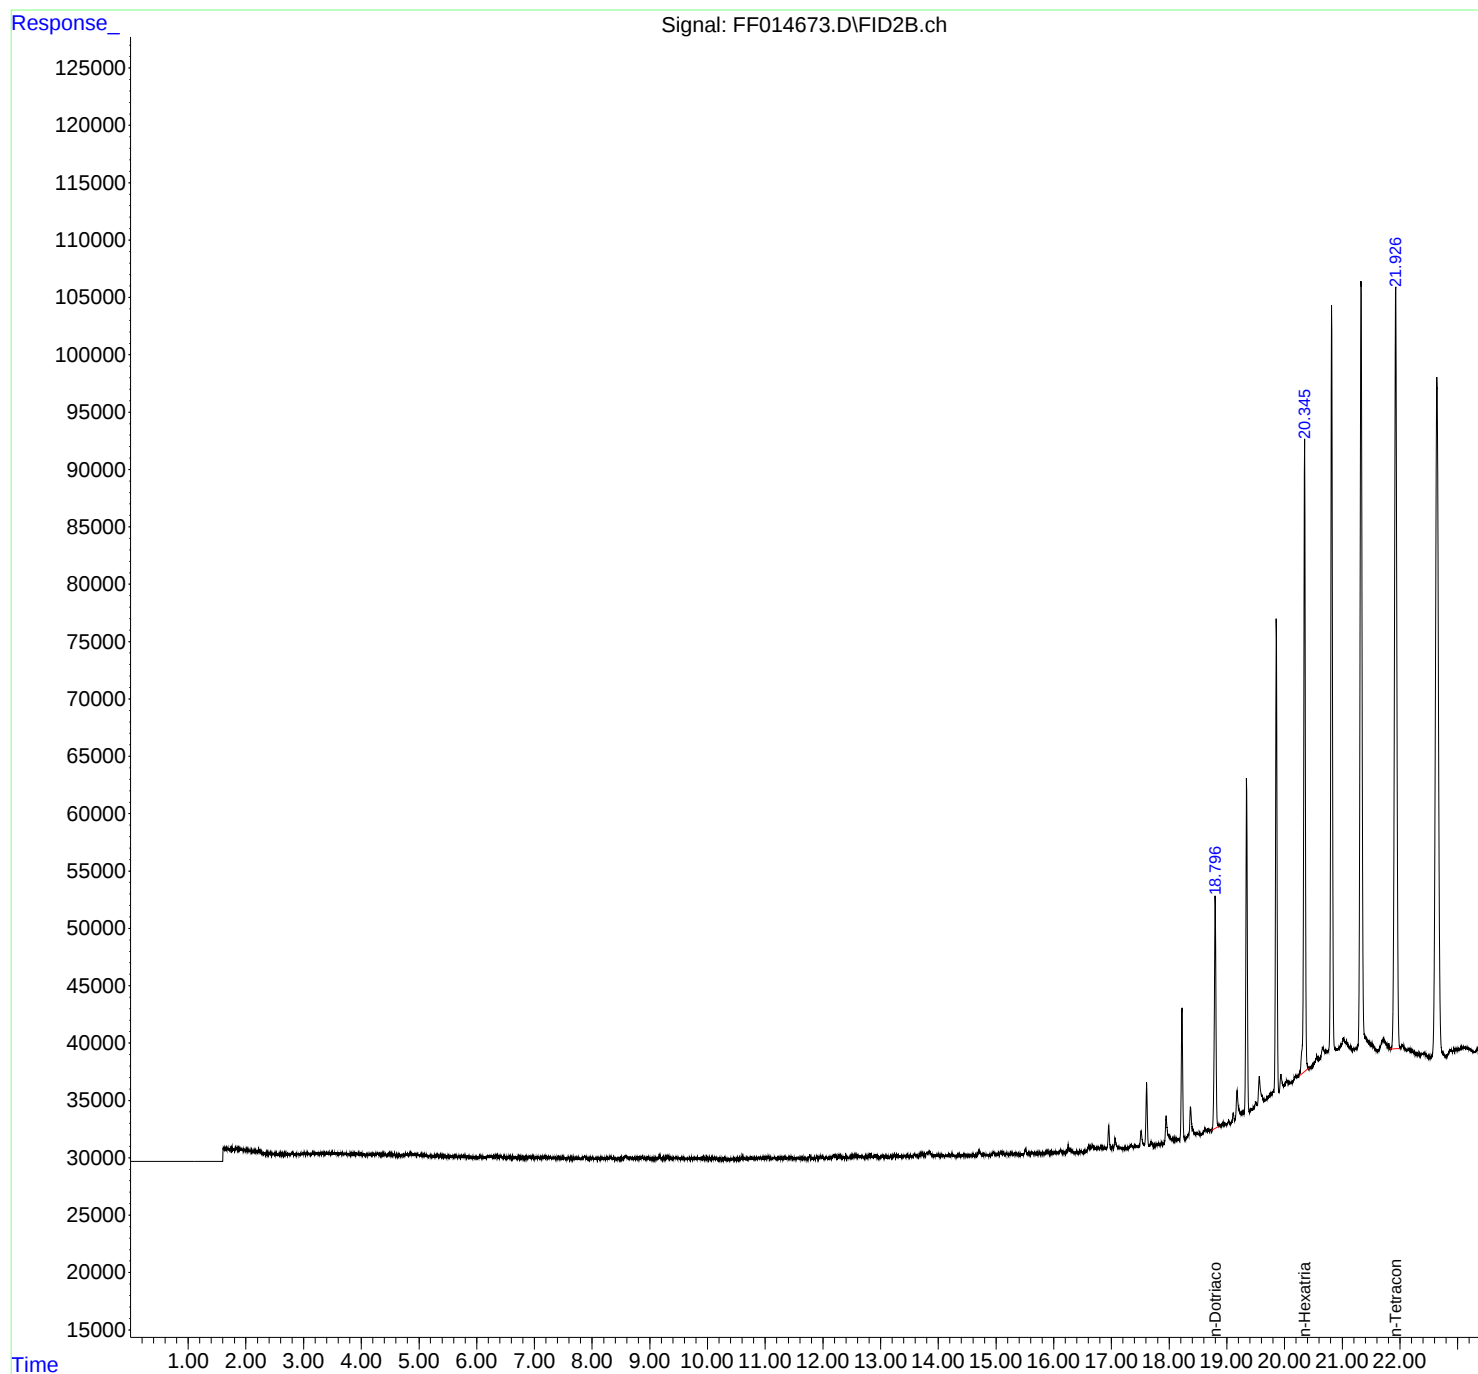


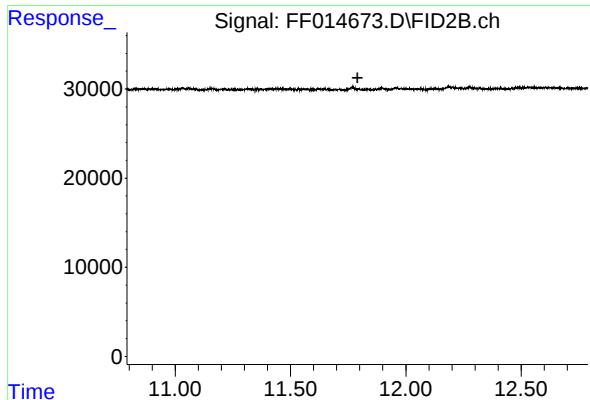

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.791 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

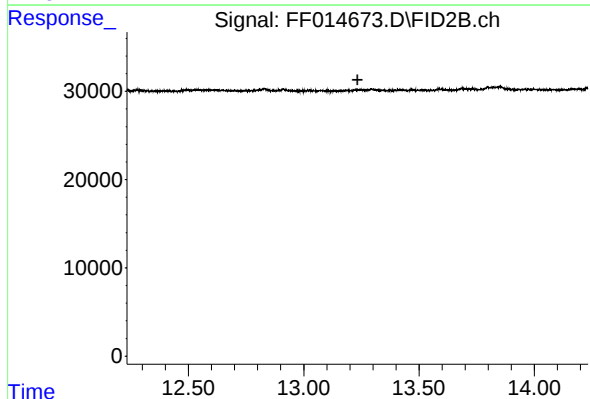


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.233 min
Response: 0
Conc: N.D.

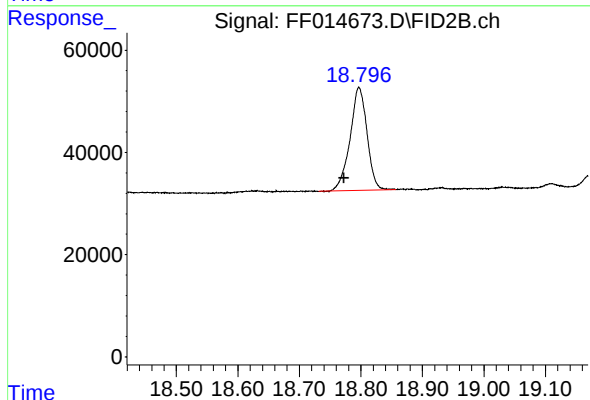


#18 n-Dotriacontane (C32)

R.T.: 18.797 min
Delta R.T.: 0.024 min
Response: 387548
Conc: 2.53 ug/ml

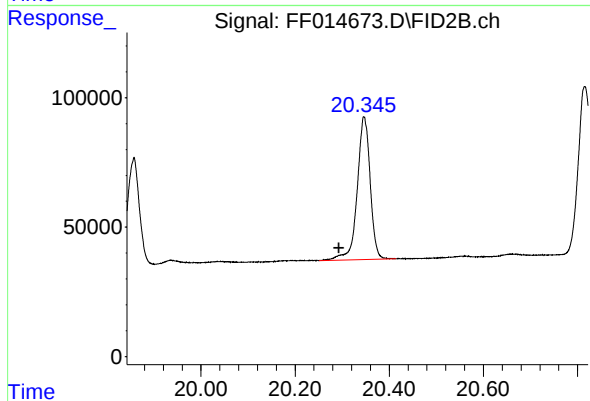

#20 n-Hexatriacontane (C36)

R.T.: 20.346 min
Delta R.T.: 0.053 min
Response: 1056518
Conc: 10.21 ug/ml

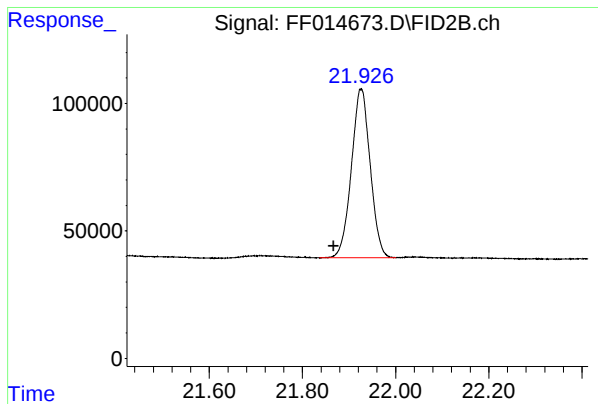

#22 n-Tetracontane (C40)

R.T.: 21.926 min
Delta R.T.: 0.059 min
Response: 1851676
Conc: 23.66 ug/ml

Instrument :

FID_F

ClientSampleId :