

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101518\
 Data File : FF002408.D
 Signal(s) : FID2B.ch
 Acq On : 15 Oct 2018 11:10
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 15 14:05:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.655	6630806	47.707 ug/ml
Target Compounds			
2) N-DECANE	4.385	7251296	47.470 ug/ml
3) N-DODECANE	6.407	7348772	47.459 ug/ml
4) N-TETRADECANE	8.201	7431339	47.490 ug/ml
5) N-HEXADECANE	9.801	7505453	47.754 ug/ml
6) N-OCTADECANE	11.244	7584911	47.727 ug/ml
7) N-EICOSANE	12.555	7553182	47.688 ug/ml
8) N-DOCOSANE	13.755	7518320	47.655 ug/ml
10) N-TETRACOSANE	14.859	7445698	47.591 ug/ml
11) N-HEXACOSANE	15.881	7401323	47.531 ug/ml
12) N-OCTACOSANE	16.833	7325776	47.228 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101518\
Data File : FF002408.D
Signal(s) : FID2B.ch
Acq On : 15 Oct 2018 11:10
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 15 14:05:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

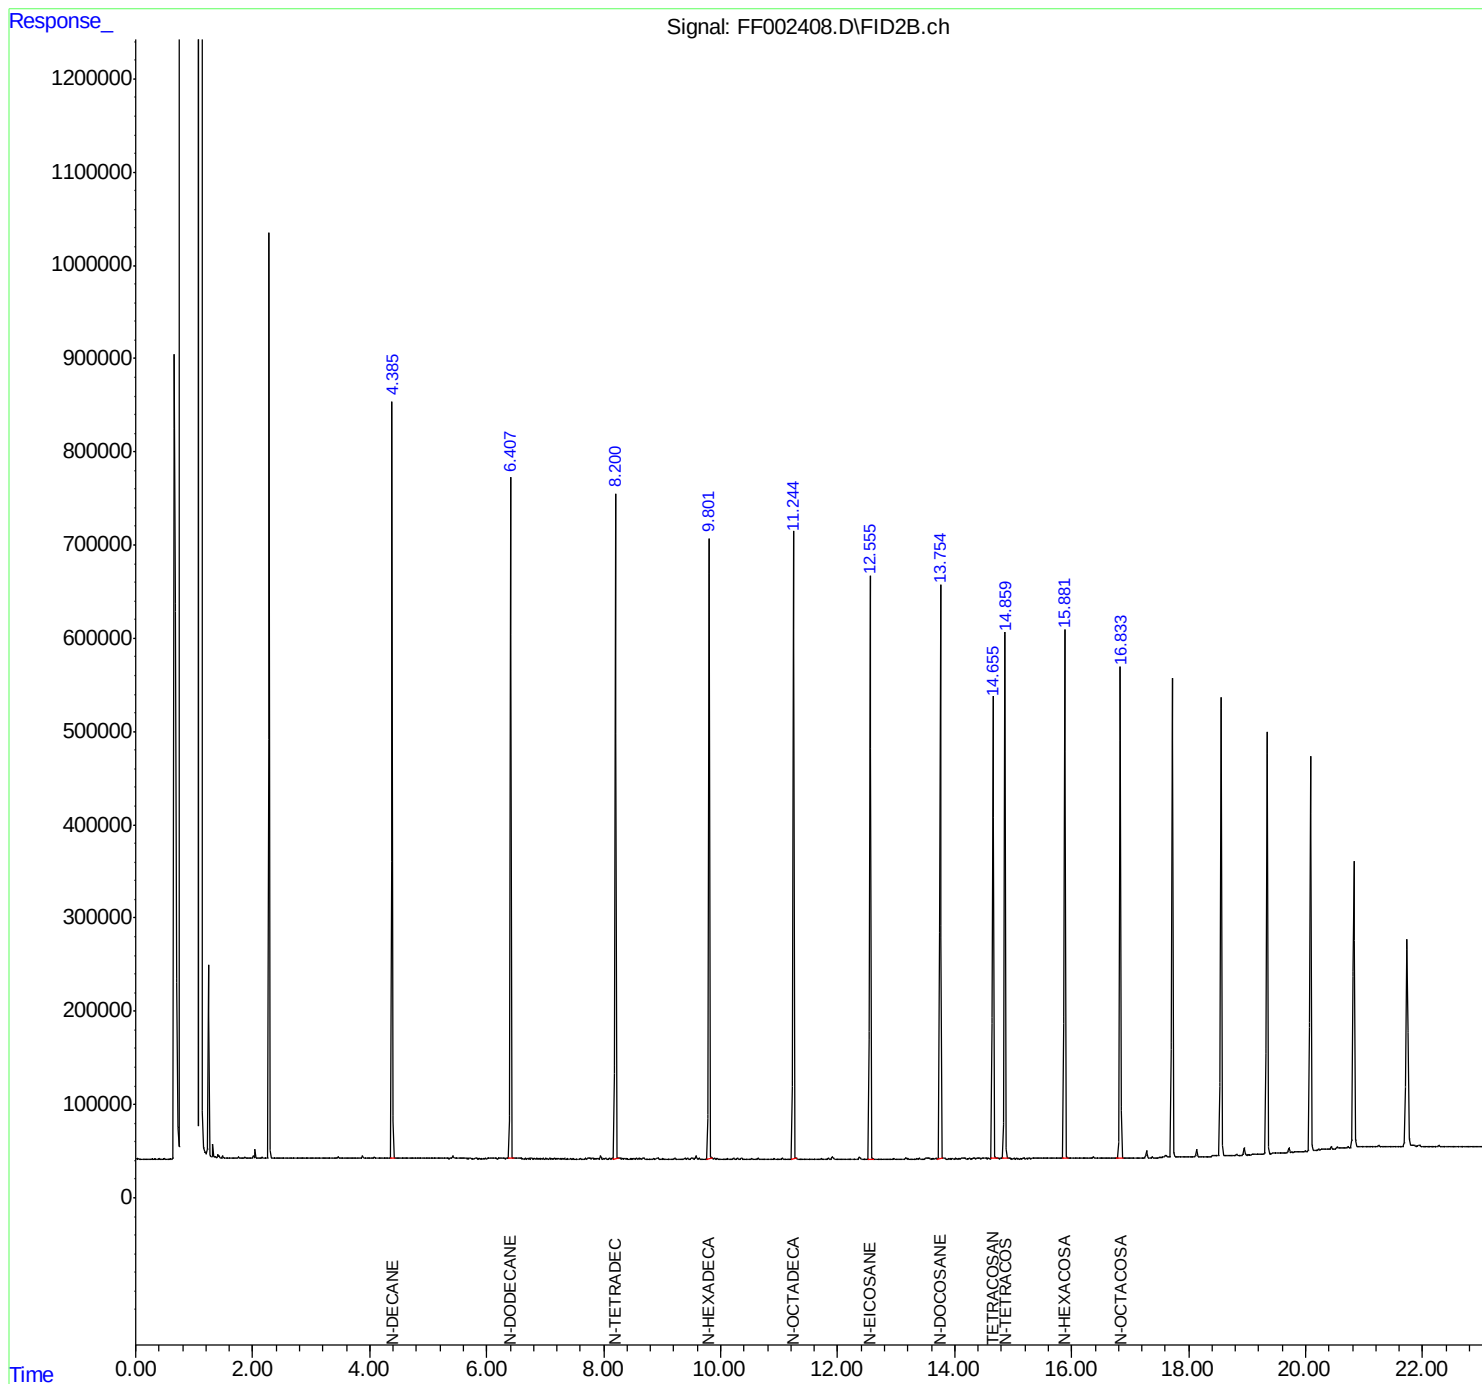

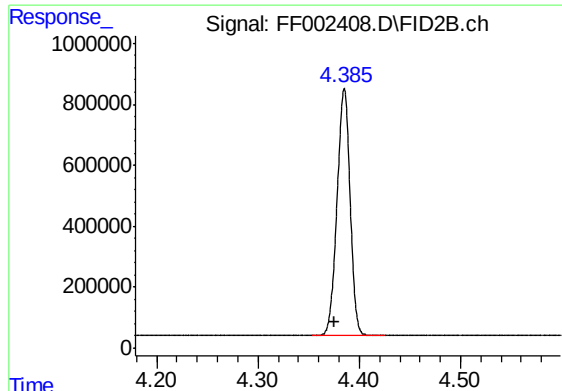


#2 N-DECANE

R.T.: 4.385 min
Delta R.T.: 0.010 min
Response: 7251296
Conc: 47.47 ug/ml

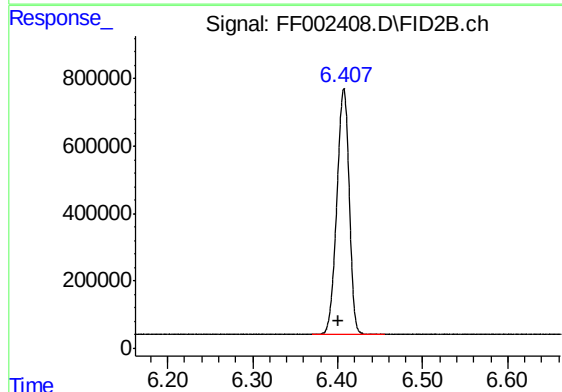


#3 N-DODECANE

R.T.: 6.407 min
Delta R.T.: 0.007 min
Response: 7348772
Conc: 47.46 ug/ml

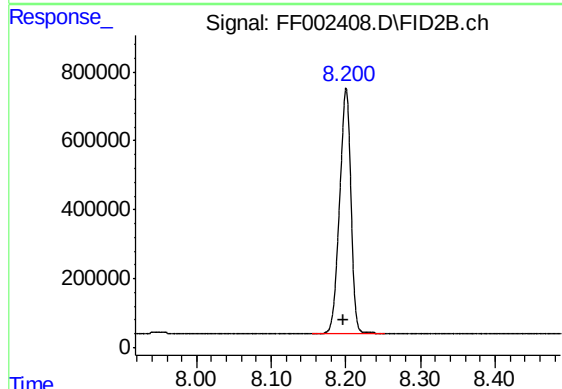


#4 N-TETRADECANE

R.T.: 8.201 min
Delta R.T.: 0.004 min
Response: 7431339
Conc: 47.49 ug/ml

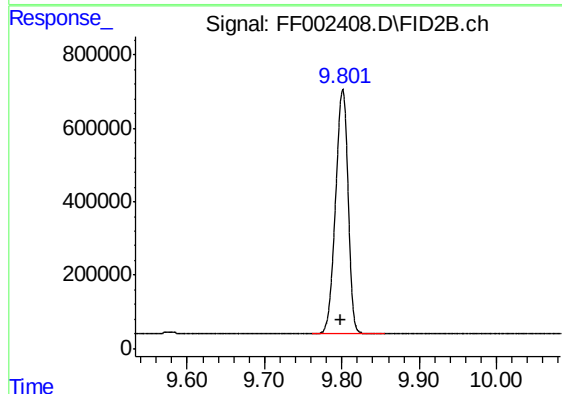


#5 N-HEXADECANE

R.T.: 9.801 min
Delta R.T.: 0.002 min
Response: 7505453
Conc: 47.75 ug/ml

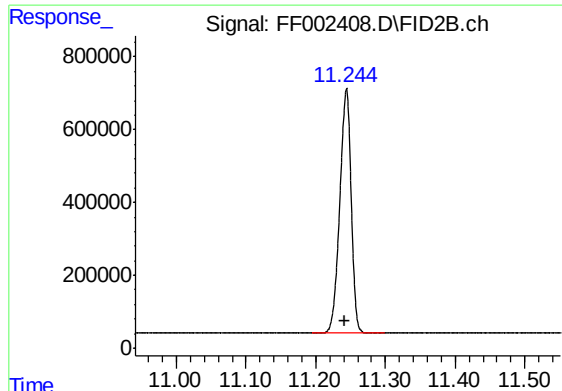


#6 N-OCTADECANE

R.T.: 11.244 min
Delta R.T.: 0.002 min
Response: 7584911
Conc: 47.73 ug/ml

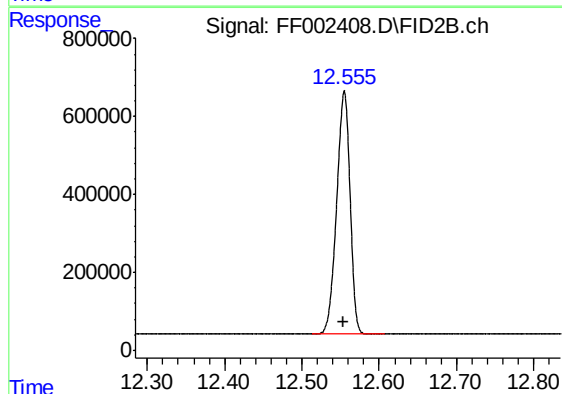


#7 N-EICOSANE

R.T.: 12.555 min
Delta R.T.: 0.000 min
Response: 7553182
Conc: 47.69 ug/ml

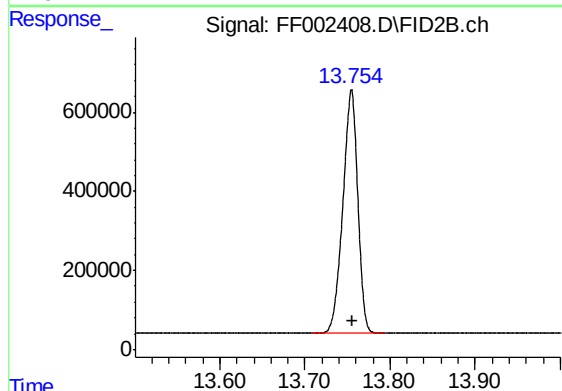


#8 N-DOCOSANE

R.T.: 13.755 min
Delta R.T.: 0.000 min
Response: 7518320
Conc: 47.66 ug/ml

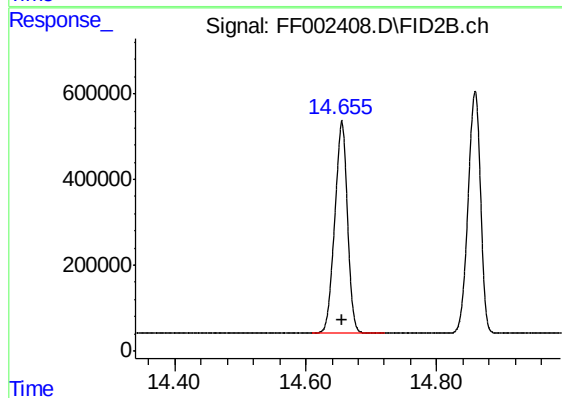


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.655 min
Delta R.T.: -0.001 min
Response: 6630806
Conc: 47.71 ug/ml

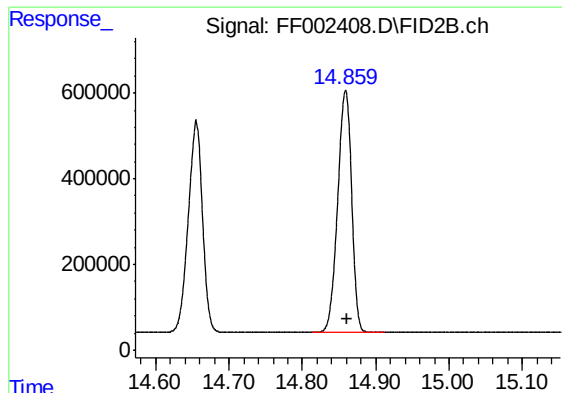


#10 N-TETRACOSANE

R.T.: 14.859 min
Delta R.T.: -0.003 min
Response: 7445698
Conc: 47.59 ug/ml

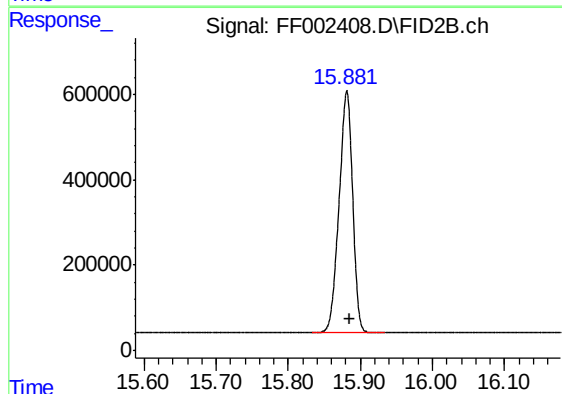

#11 N-HEXACOSANE

R.T.: 15.881 min
Delta R.T.: -0.003 min
Response: 7401323
Conc: 47.53 ug/ml

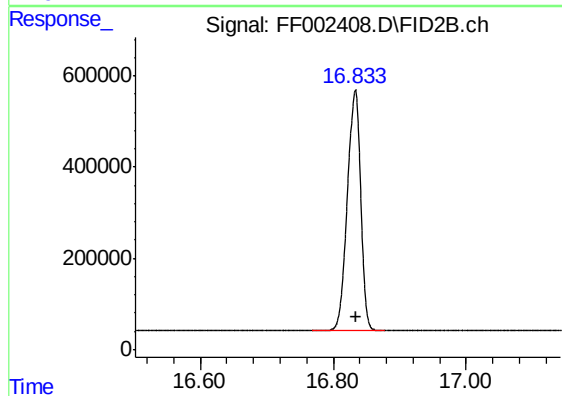

#12 N-OCTACOSANE

R.T.: 16.833 min
Delta R.T.: -0.002 min
Response: 7325776
Conc: 47.23 ug/ml