

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
 Data File : FF009142.D
 Signal(s) : FID2B.ch
 Acq On : 15 Oct 2021 10:49
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 16 00:15:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
 Quant Title :
 QLast Update : Fri Oct 08 02:25:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.482	2987308	23.514 ug/ml
12) N-OCTACOSANE	16.881	2991766	25.557 ug/ml
13) N-TRIACONTANE	17.764	152181	1.349 ug/ml
14) N-DOTRIACONTANE	18.593	205109	1.942 ug/ml
15) N-TETRATRIACONTANE	19.374	177031	1.811 ug/ml
16) N-HEXATRIACONTANE	20.111	221689	2.494 ug/ml
17) N-OCTATRIACONTANE	20.850	169409	2.075 ug/ml
18) N-TETRACONTANE	21.766	251523	3.096 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
Data File : FF009142.D
Signal(s) : FID2B.ch
Acq On : 15 Oct 2021 10:49
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:15:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

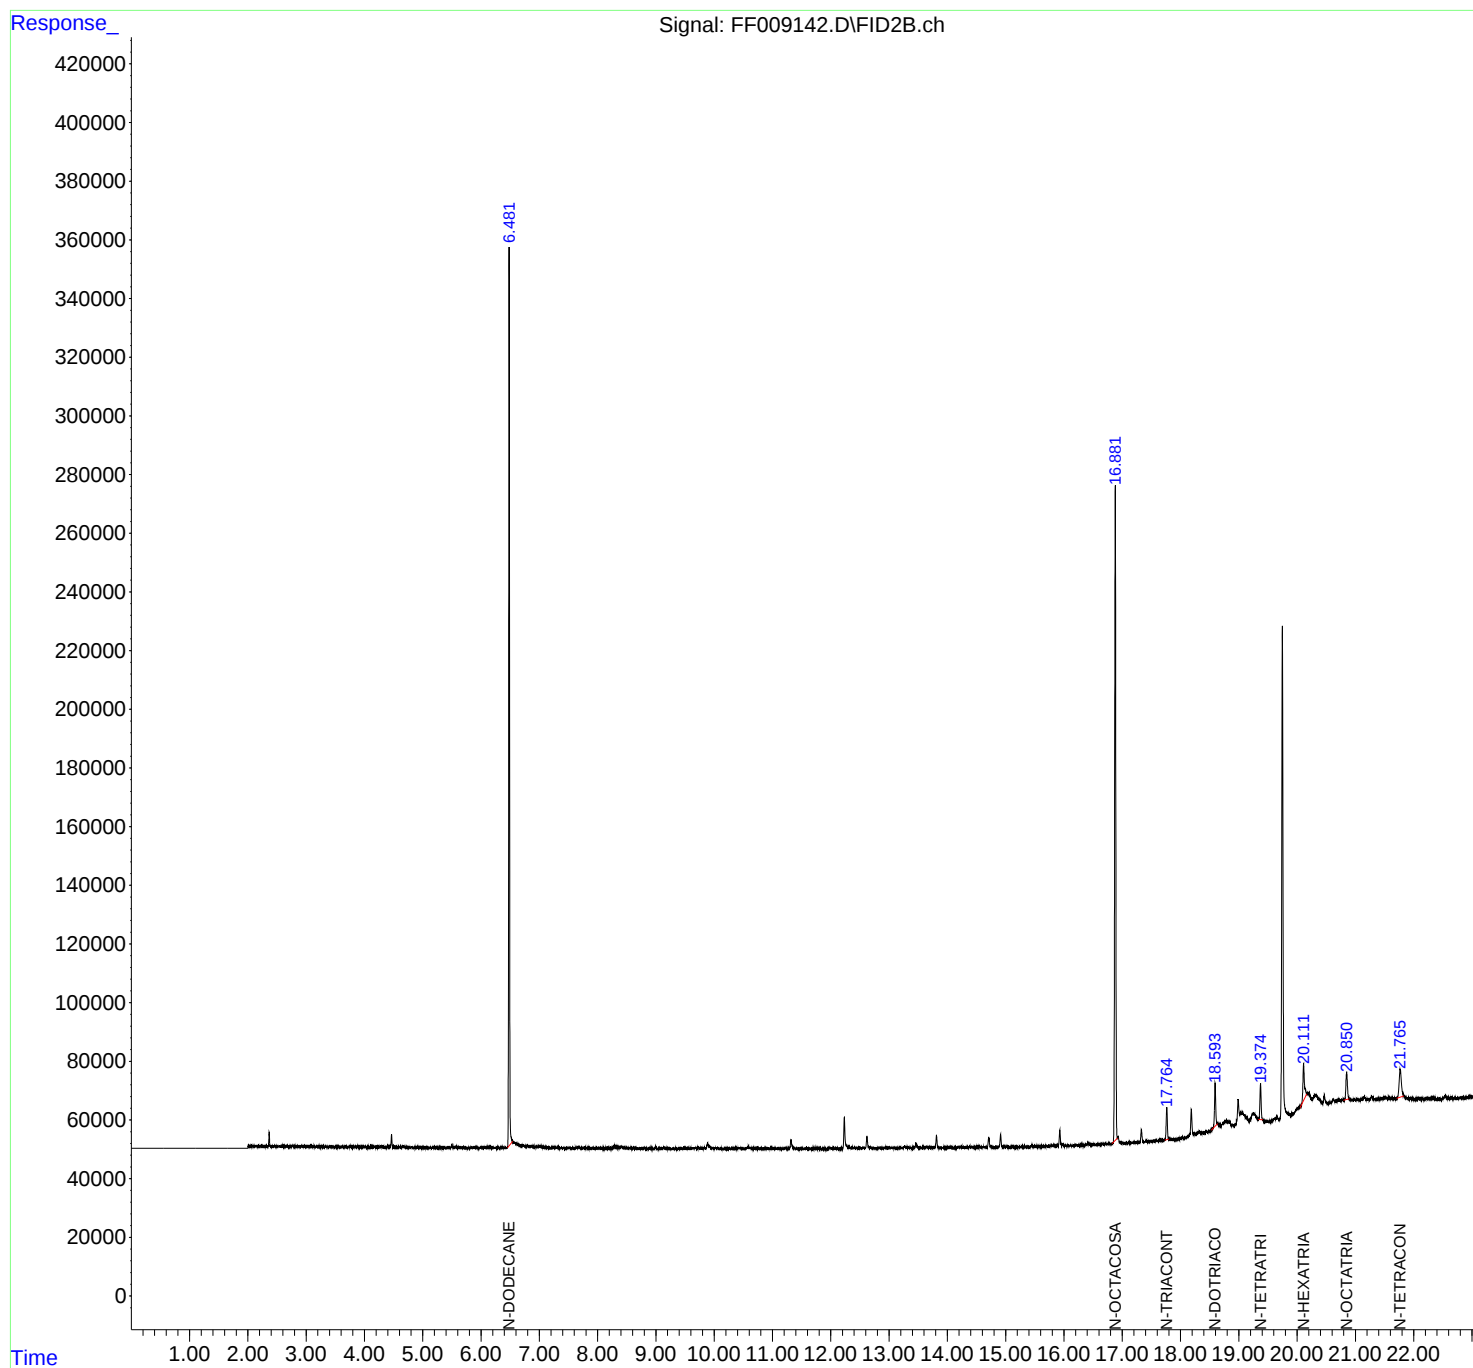


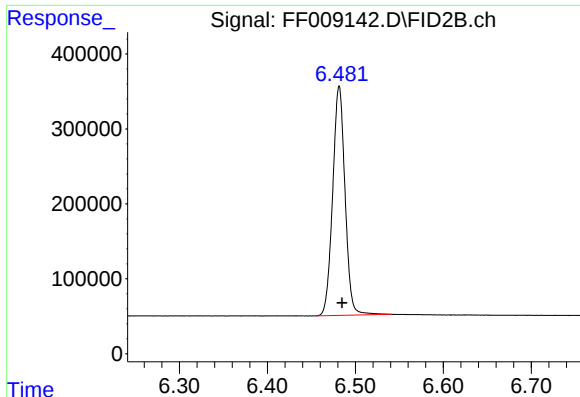

#3 N-DODECANE


R.T.: 6.482 min
Delta R.T.: -0.003 min
Response: 2987308
Conc: 23.51 ug/ml

Instrument :
FID_F
ClientSampleId :

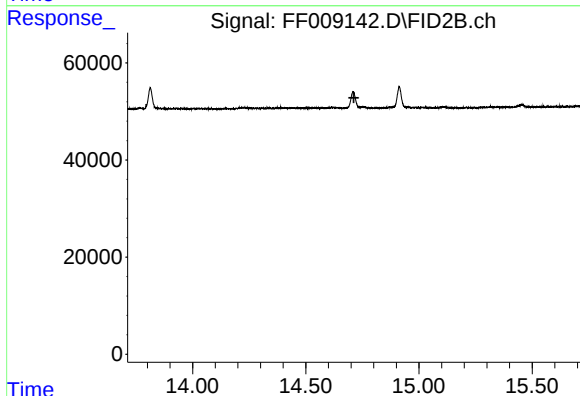


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.

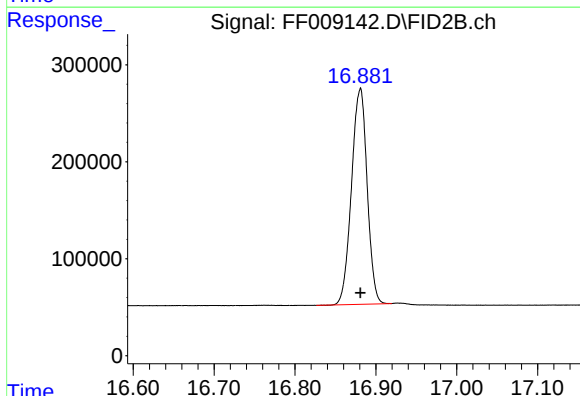


#12 N-OCTACOSANE

R.T.: 16.881 min
Delta R.T.: 0.000 min
Response: 2991766
Conc: 25.56 ug/ml

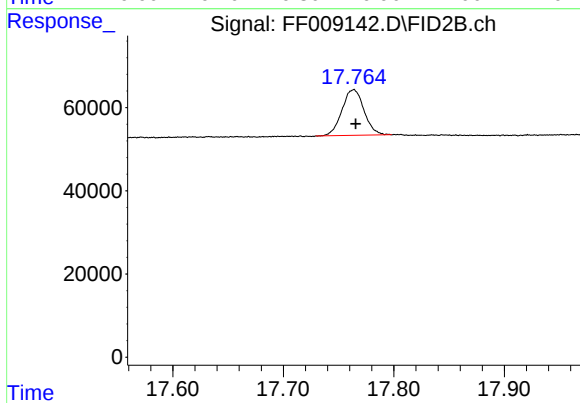

#13 N-TRIACONTANE


R.T.: 17.764 min
Delta R.T.: -0.001 min
Response: 152181
Conc: 1.35 ug/ml

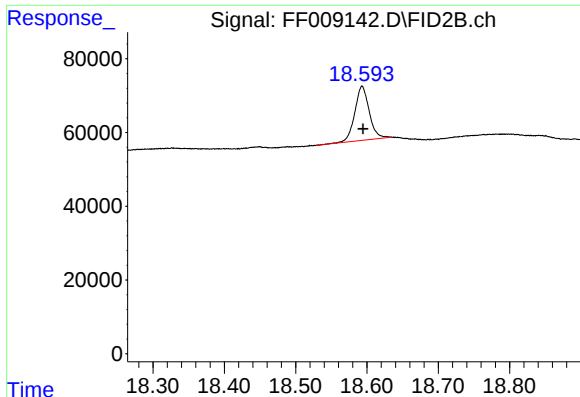

#14 N-DOTRIACONTANE


R.T.: 18.593 min
Delta R.T.: -0.002 min
Response: 205109
Conc: 1.94 ug/ml

Instrument :
FID_F
ClientSampleId :

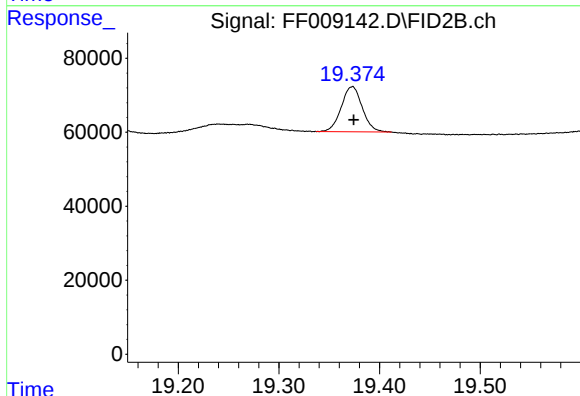


#15 N-TETRATRIACONTANE

R.T.: 19.374 min
Delta R.T.: -0.001 min
Response: 177031
Conc: 1.81 ug/ml

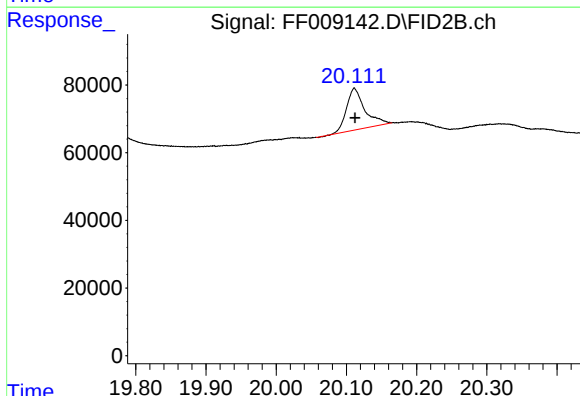


#16 N-HEXATRIACONTANE

R.T.: 20.111 min
Delta R.T.: -0.001 min
Response: 221689
Conc: 2.49 ug/ml

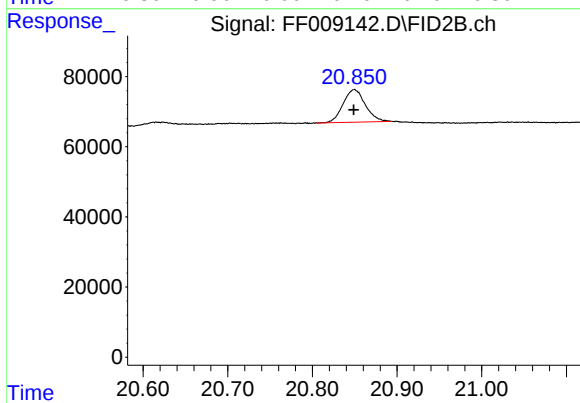

#17 N-OCTATRIACONTANE

R.T.: 20.850 min
Delta R.T.: 0.000 min
Response: 169409
Conc: 2.08 ug/ml

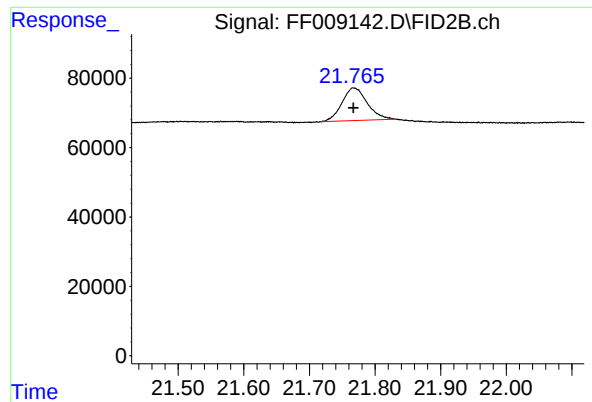

#18 N-TETRACONTANE

R.T.: 21.766 min
Delta R.T.: -0.001 min
Response: 251523
Conc: 3.10 ug/ml

Instrument :
FID_F
ClientSampleId :