

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
Data File : FF009143.D
Signal(s) : FID2B.ch
Acq On : 15 Oct 2021 13:23
Operator : AJ\MA
Sample : PB139876BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:16:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	2140261	19.518 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.600	418510	3.963 ug/ml
16) N-HEXATRIACONTANE	20.144	959604	10.793 ug/ml
18) N-TETRACONTANE	21.784	2019158	24.854 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
Data File : FF009143.D
Signal(s) : FID2B.ch
Acq On : 15 Oct 2021 13:23
Operator : AJ\MA
Sample : PB139876BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:16:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

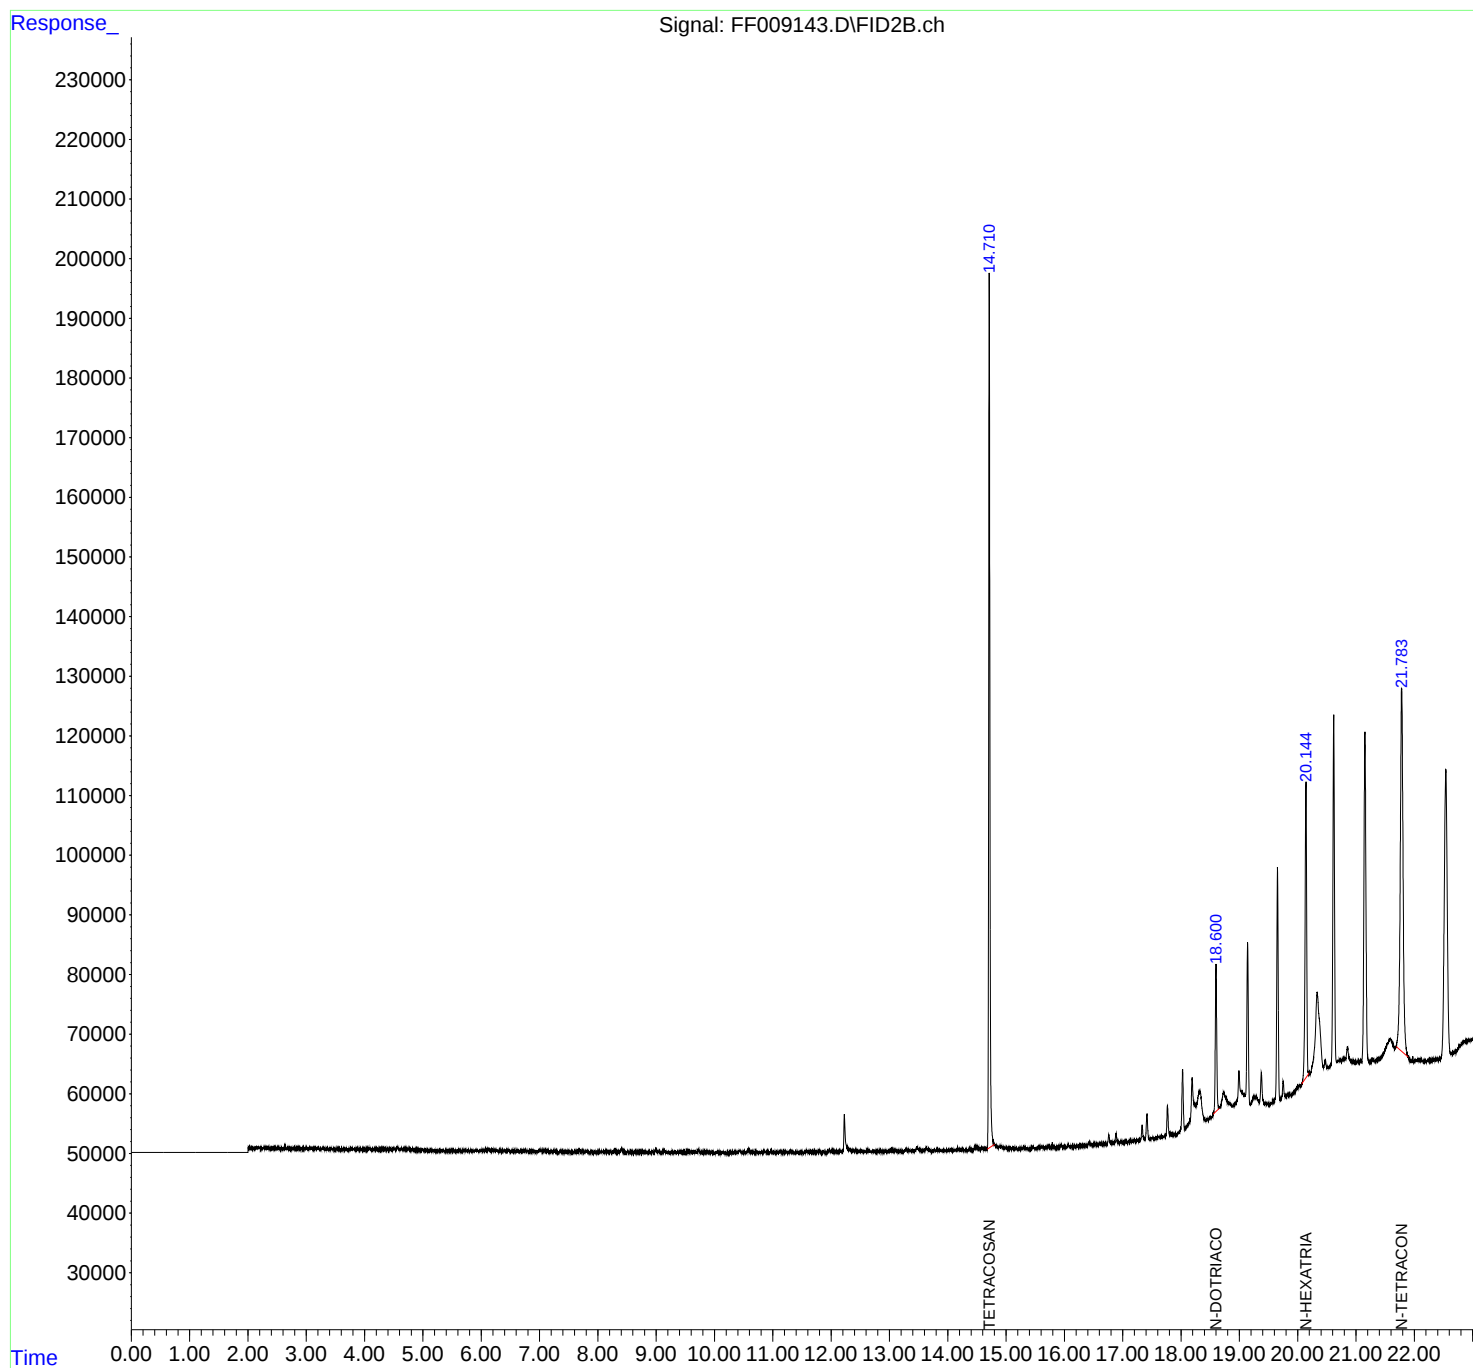


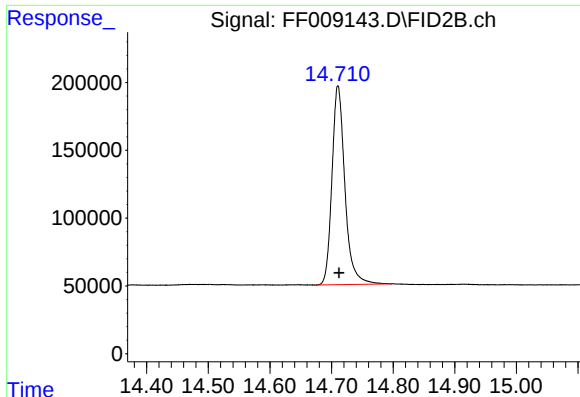

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.711 min
Delta R.T.: -0.002 min
Response: 2140261
Conc: 19.52 ug/ml

Instrument :
FID_F
ClientSampleId :

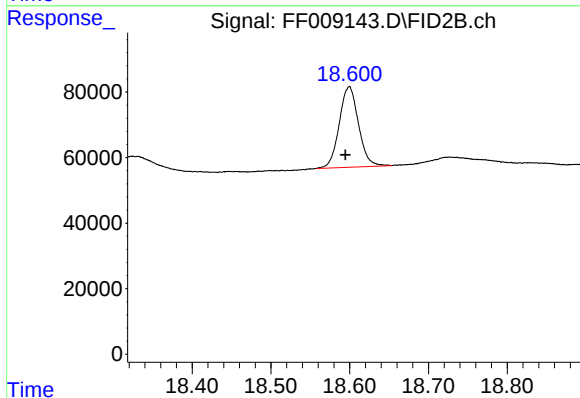


#14 N-DOTRIACONTANE

R.T.: 18.600 min
Delta R.T.: 0.005 min
Response: 418510
Conc: 3.96 ug/ml

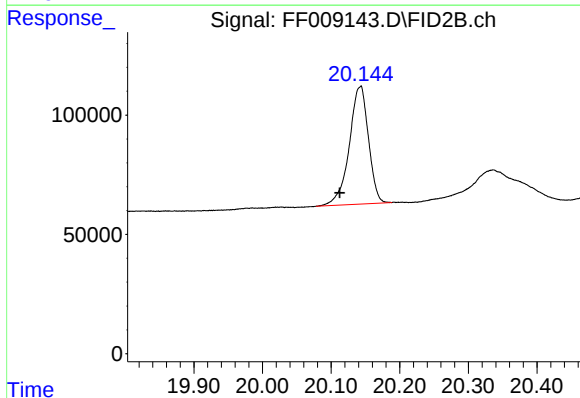

#16 N-HEXATRIACONTANE

R.T.: 20.144 min
Delta R.T.: 0.032 min
Response: 959604
Conc: 10.79 ug/ml

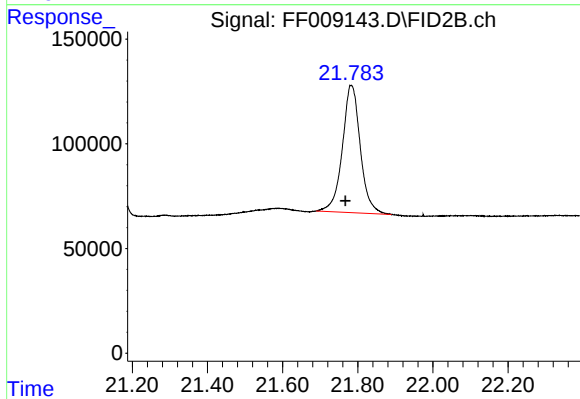

#18 N-TETRACONTANE

R.T.: 21.784 min
Delta R.T.: 0.017 min
Response: 2019158
Conc: 24.85 ug/ml