

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
Data File : FF009145.D
Signal(s) : FID2B.ch
Acq On : 15 Oct 2021 14:58
Operator : AJ\MA
Sample : PB139889BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:16:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.711	2075113	18.924 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	20.142	97996	1.102 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
Data File : FF009145.D
Signal(s) : FID2B.ch
Acq On : 15 Oct 2021 14:58
Operator : AJ\MA
Sample : PB139889BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:16:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

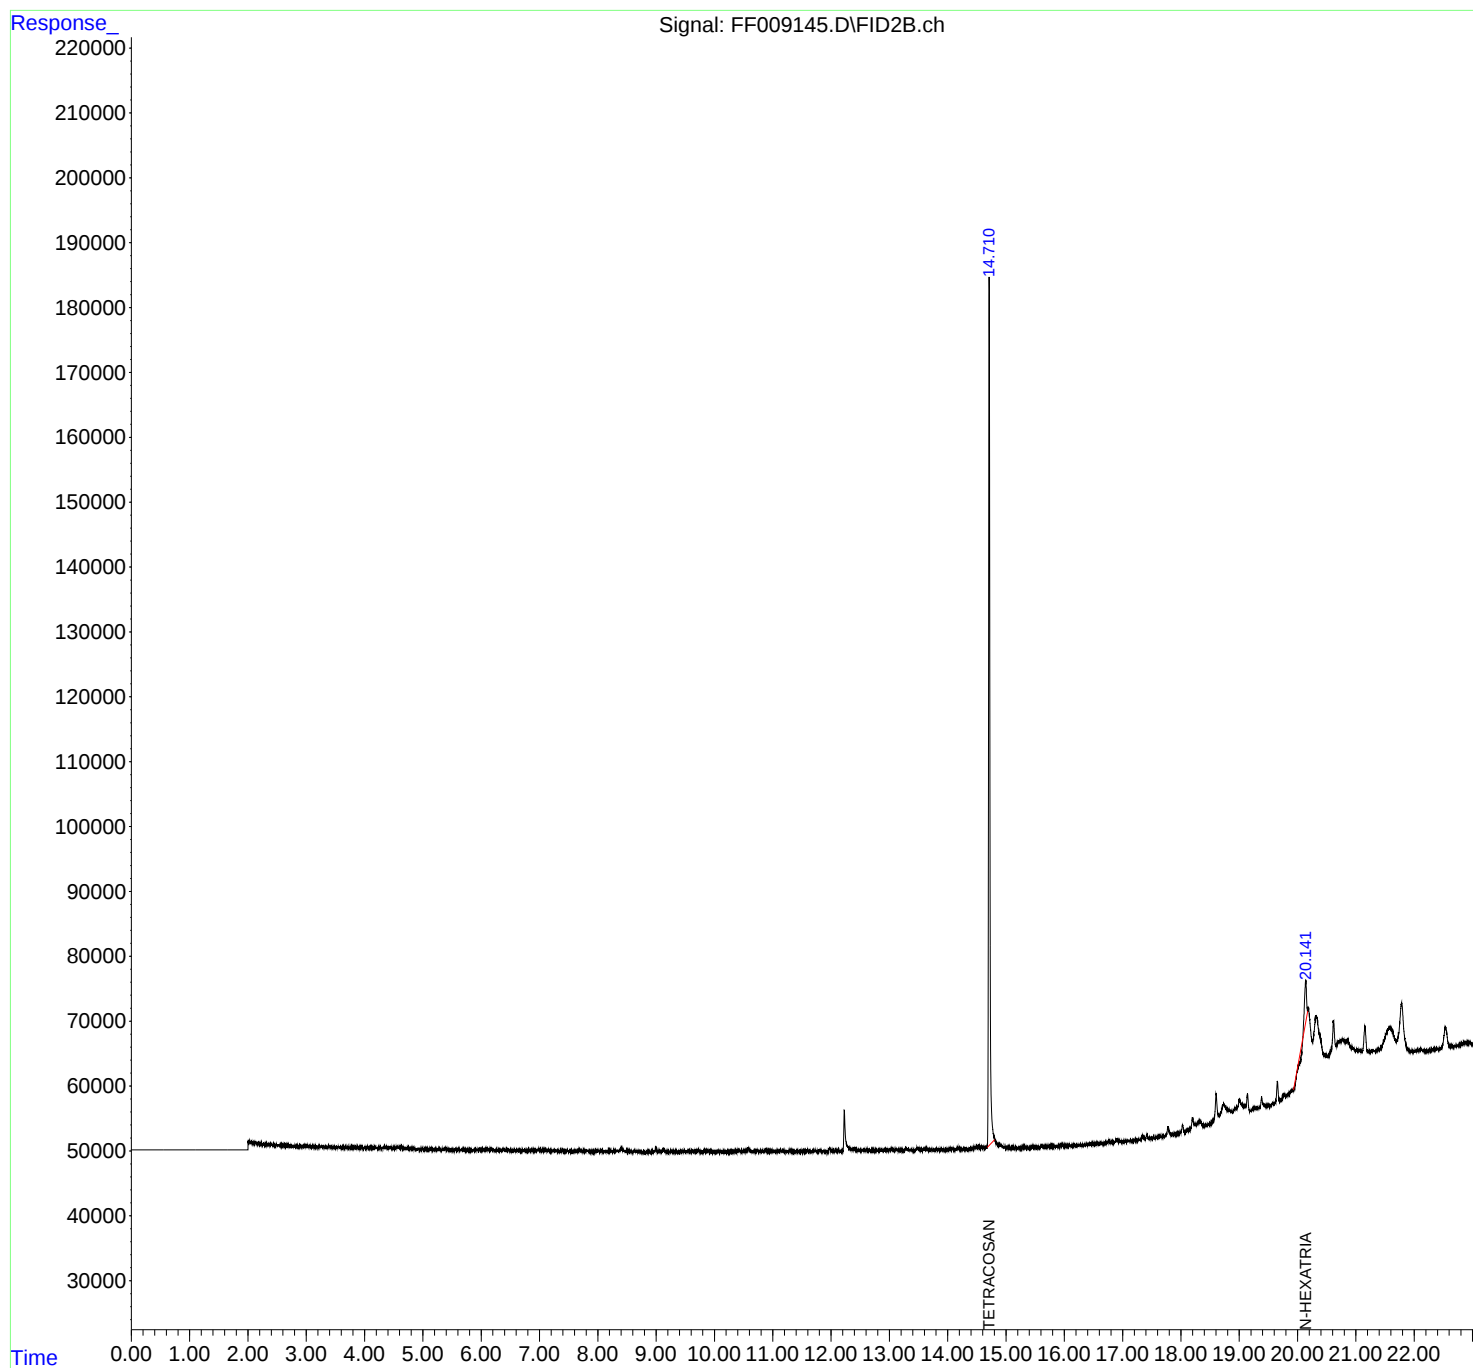


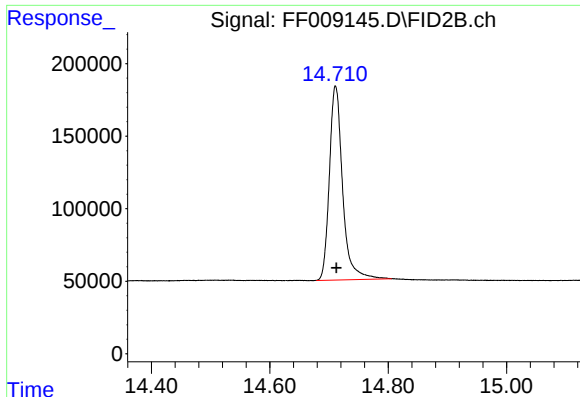

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.711 min
Delta R.T.: -0.002 min
Response: 2075113
Conc: 18.92 ug/ml

Instrument :
FID_F
ClientSampleId :

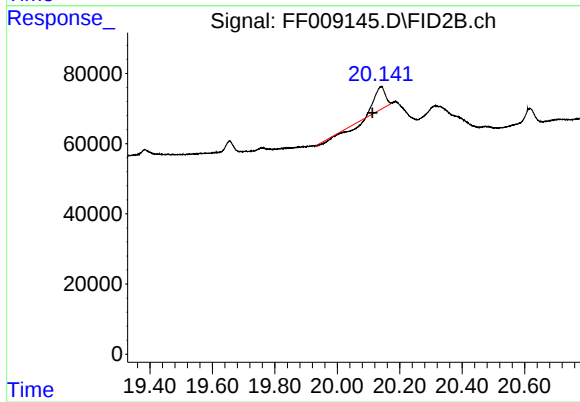

#16 N-HEXATRIACONTANE

R.T.: 20.142 min
Delta R.T.: 0.029 min
Response: 97996
Conc: 1.10 ug/ml