

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
 Data File : FF009149.D
 Signal(s) : FID2B.ch
 Acq On : 15 Oct 2021 17:03
 Operator : AJ\MA
 Sample : PB139920BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 16 00:17:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
 Quant Title :
 QLast Update : Fri Oct 08 02:25:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.710	2140450	19.520 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.143	223132	2.510 ug/ml
18) N-TETRACONTANE	21.776	506883	6.239 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
Data File : FF009149.D
Signal(s) : FID2B.ch
Acq On : 15 Oct 2021 17:03
Operator : AJ\MA
Sample : PB139920BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:17:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

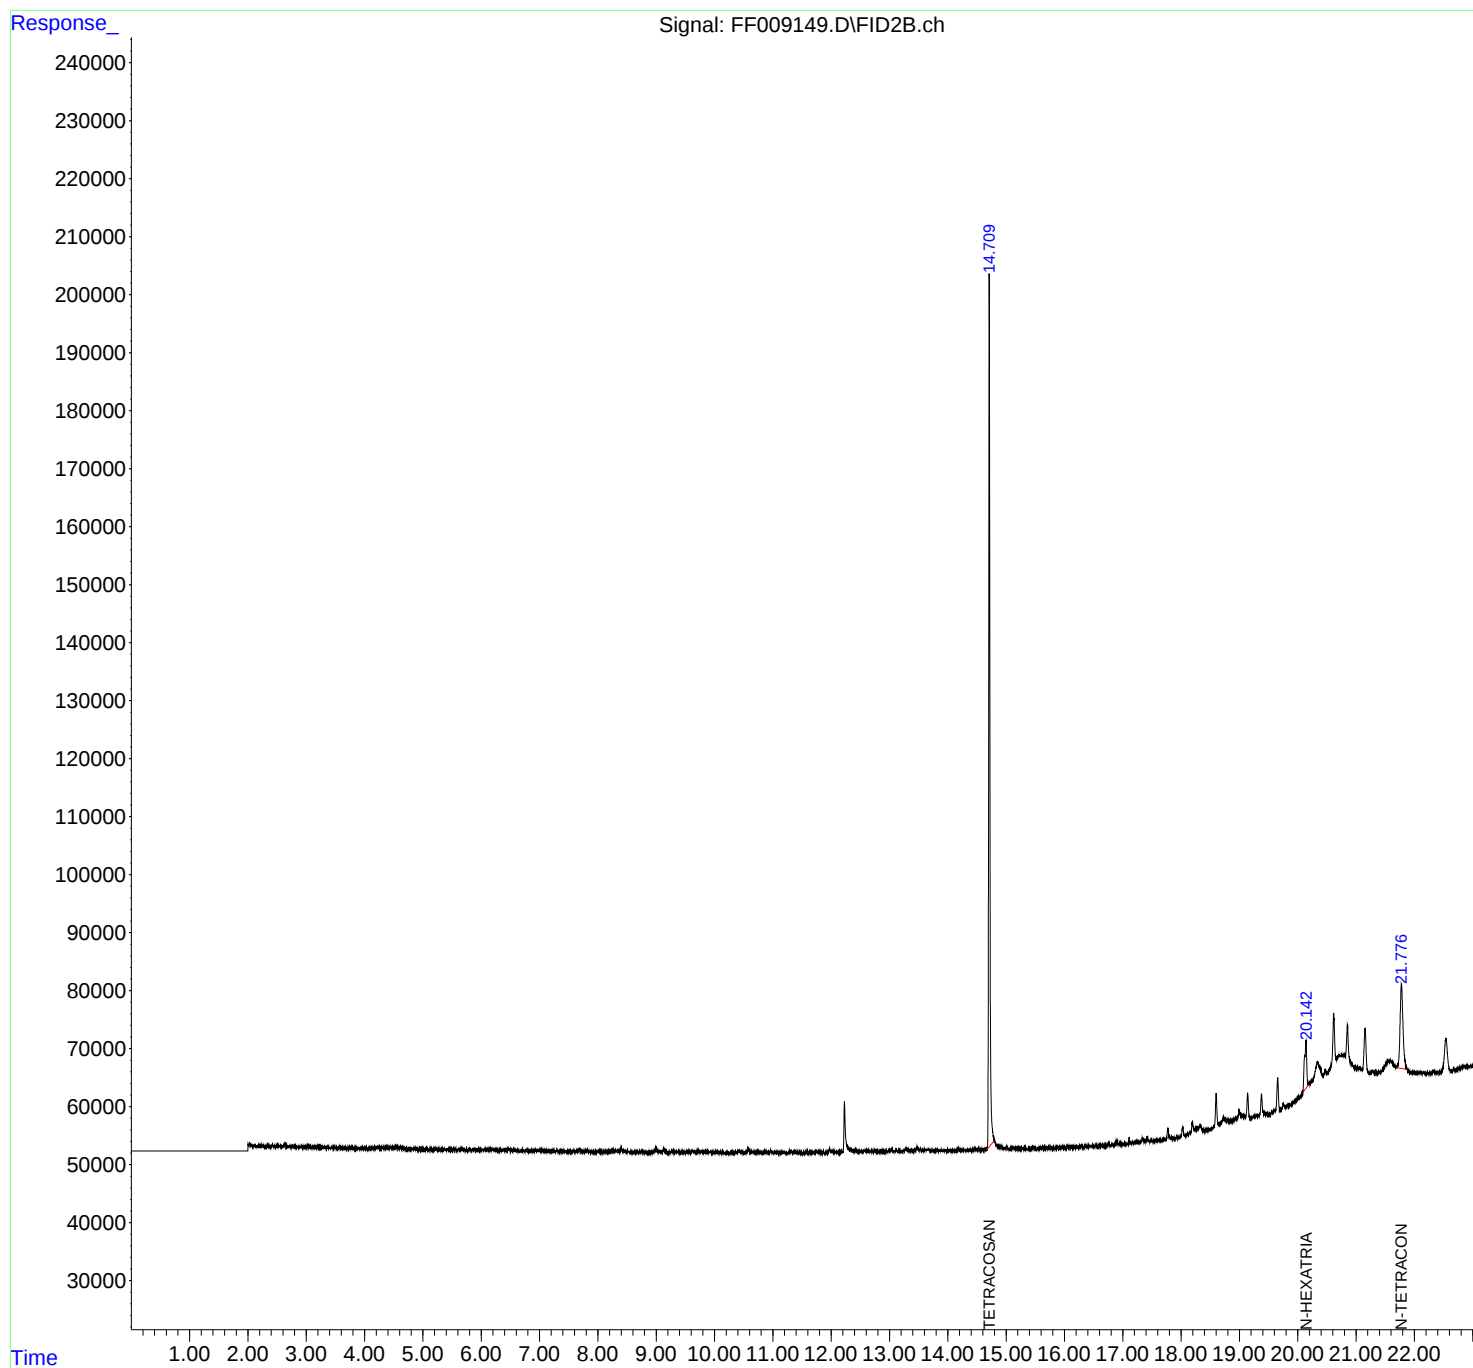


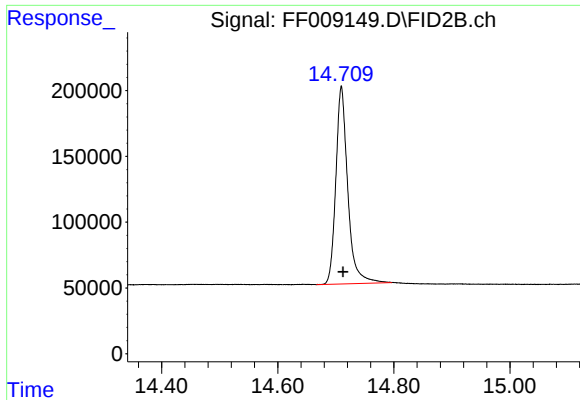

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.710 min
Delta R.T.: -0.003 min
Response: 2140450
Conc: 19.52 ug/ml

Instrument :
FID_F
ClientSampleId :

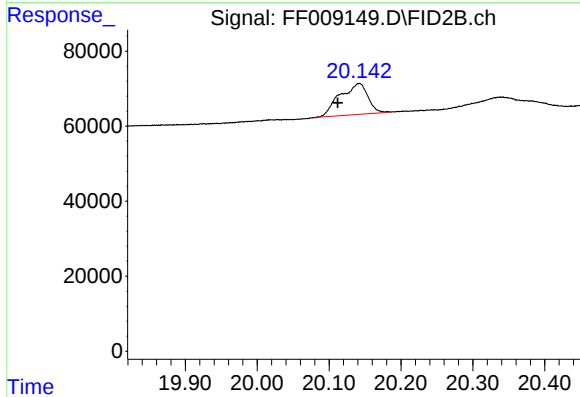

#16 N-HEXATRIACONTANE

R.T.: 20.143 min
Delta R.T.: 0.030 min
Response: 223132
Conc: 2.51 ug/ml

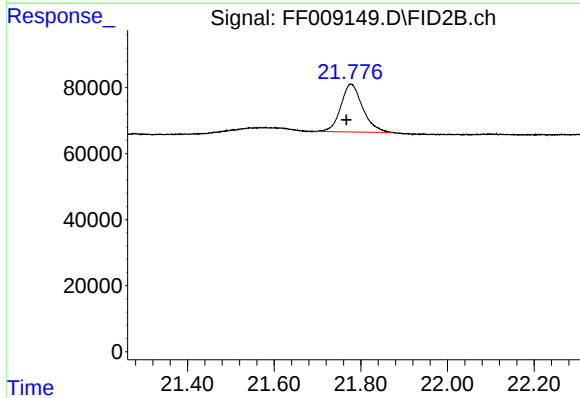

#18 N-TETRACONTANE

R.T.: 21.776 min
Delta R.T.: 0.009 min
Response: 506883
Conc: 6.24 ug/ml