

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
 Data File : FF009155.D
 Signal(s) : FID2B.ch
 Acq On : 15 Oct 2021 20:11
 Operator : AJ\MA
 Sample : M4202-02 5X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 16 00:19:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
 Quant Title :
 QLast Update : Fri Oct 08 02:25:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.713	217462	1.983 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.597	132848	1.258 ug/ml
15) N-TETRATRIACONTANE	19.372	52870	0.541 ug/ml
16) N-HEXATRIACONTANE	20.127	146907	1.652 ug/ml
18) N-TETRACONTANE	21.745	7595	0.093 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
Data File : FF009155.D
Signal(s) : FID2B.ch
Acq On : 15 Oct 2021 20:11
Operator : AJ\MA
Sample : M4202-02 5X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Oct 16 00:19:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

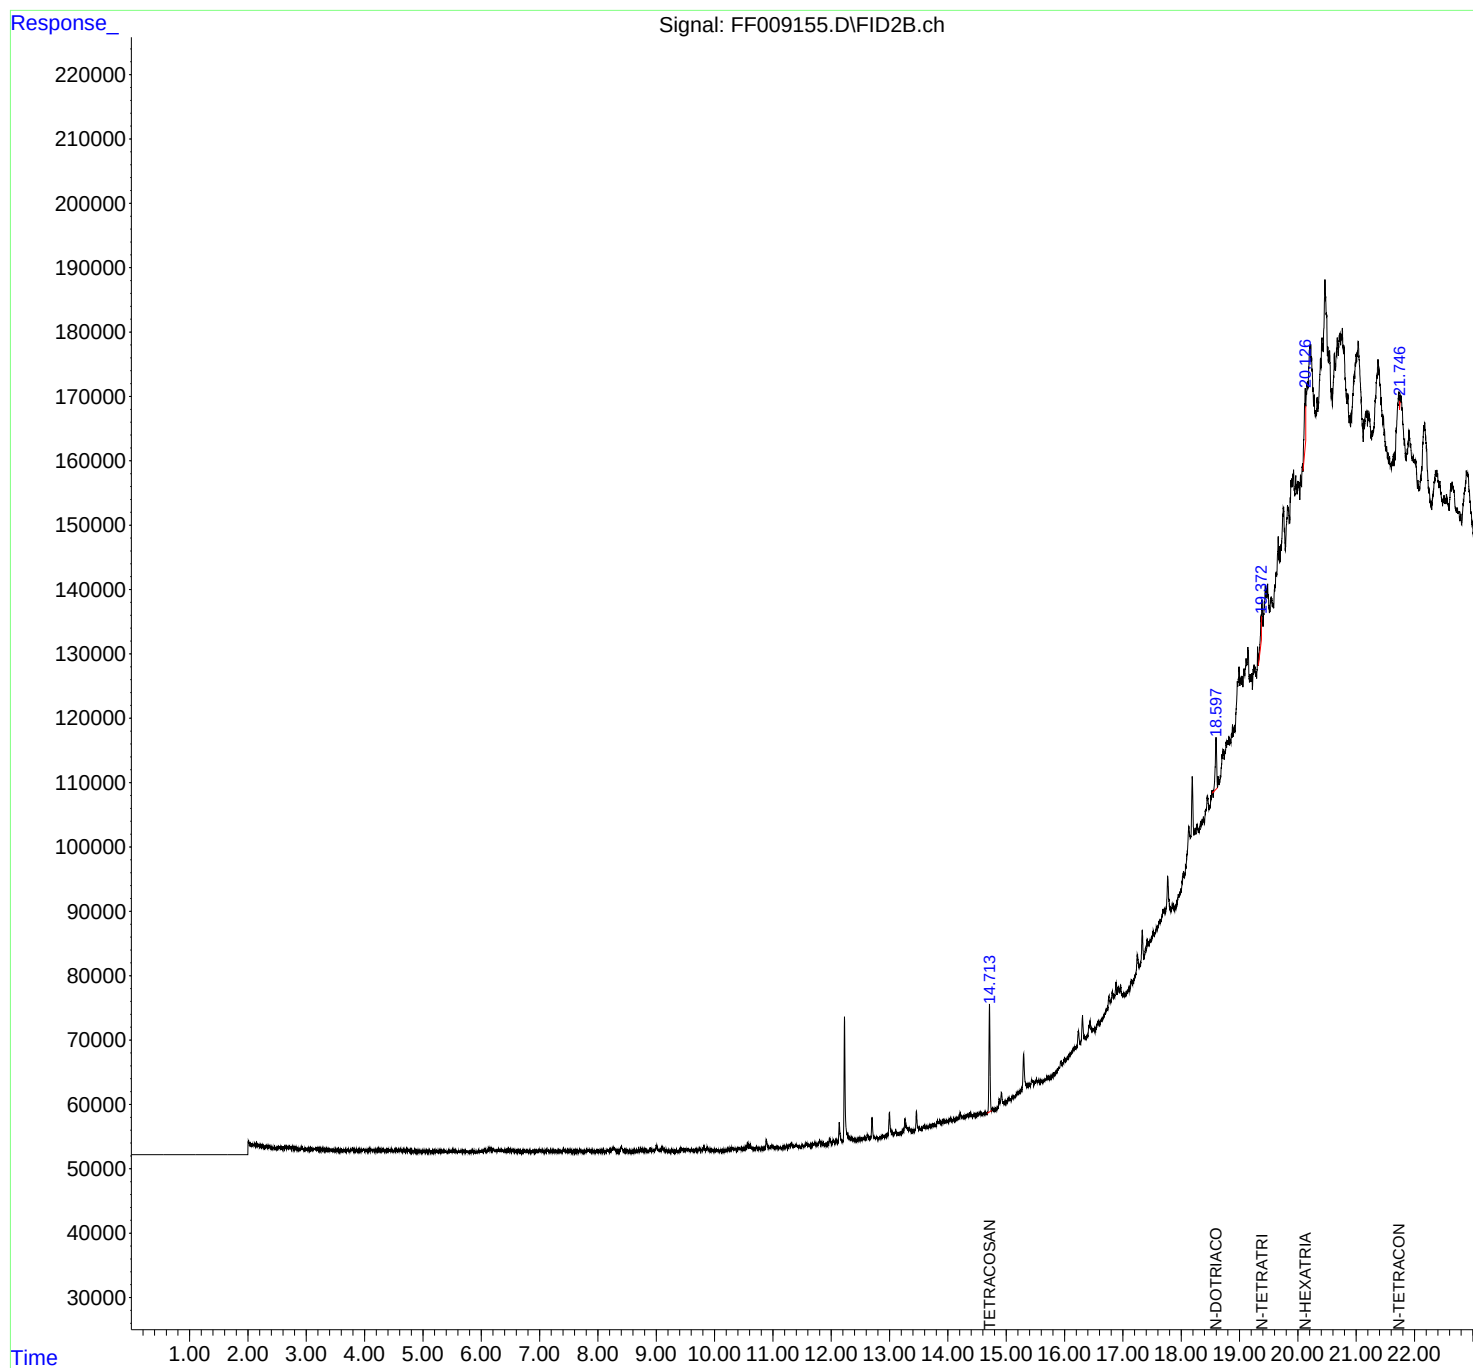


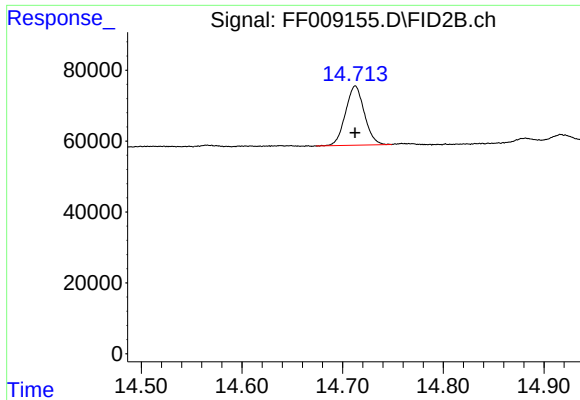

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.713 min
Delta R.T.: 0.000 min
Response: 217462
Conc: 1.98 ug/ml

Instrument :
FID_F
ClientSampleId :

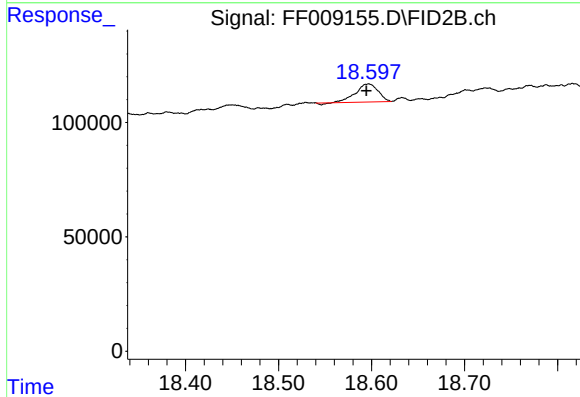


#14 N-DOTRIACONTANE

R.T.: 18.597 min
Delta R.T.: 0.003 min
Response: 132848
Conc: 1.26 ug/ml

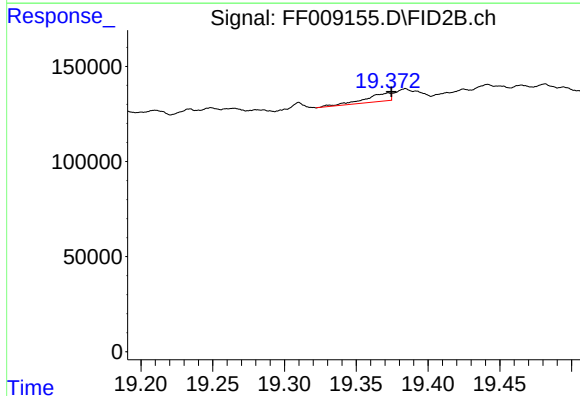


#15 N-TETRATRIACONTANE

R.T.: 19.372 min
Delta R.T.: -0.002 min
Response: 52870
Conc: 0.54 ug/ml

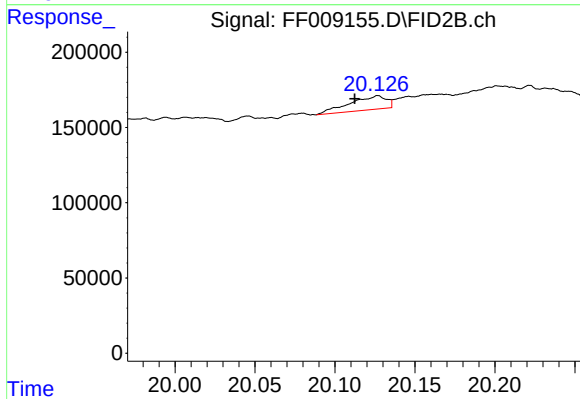

#16 N-HEXATRIACONTANE

R.T.: 20.127 min
Delta R.T.: 0.014 min
Response: 146907
Conc: 1.65 ug/ml

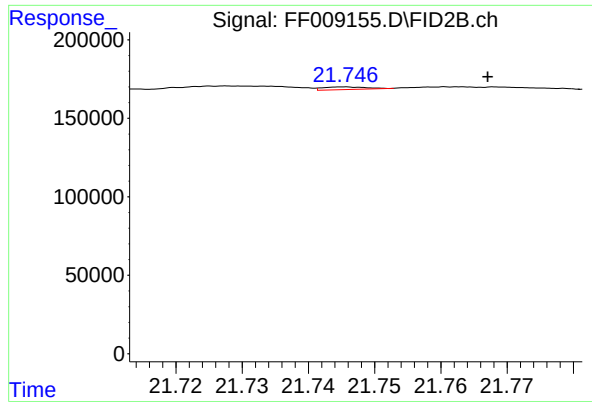

#18 N-TETRACONTANE

R.T.: 21.745 min
Delta R.T.: -0.022 min
Response: 7595
Conc: 0.09 ug/ml

Instrument :
FID_F
ClientSampleId :