

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
Data File : FF009156.D
Signal(s) : FID2B.ch
Acq On : 15 Oct 2021 20:42
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:19:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.603	107845	1.021 ug/ml
15)	N-TETRATRIACONTANE	19.383	32445	0.332 ug/ml
16)	N-HEXATRIACONTANE	20.145	293865	3.305 ug/ml
18)	N-TETRACONTANE	21.783	292367	3.599 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101521\
Data File : FF009156.D
Signal(s) : FID2B.ch
Acq On : 15 Oct 2021 20:42
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 16 00:19:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

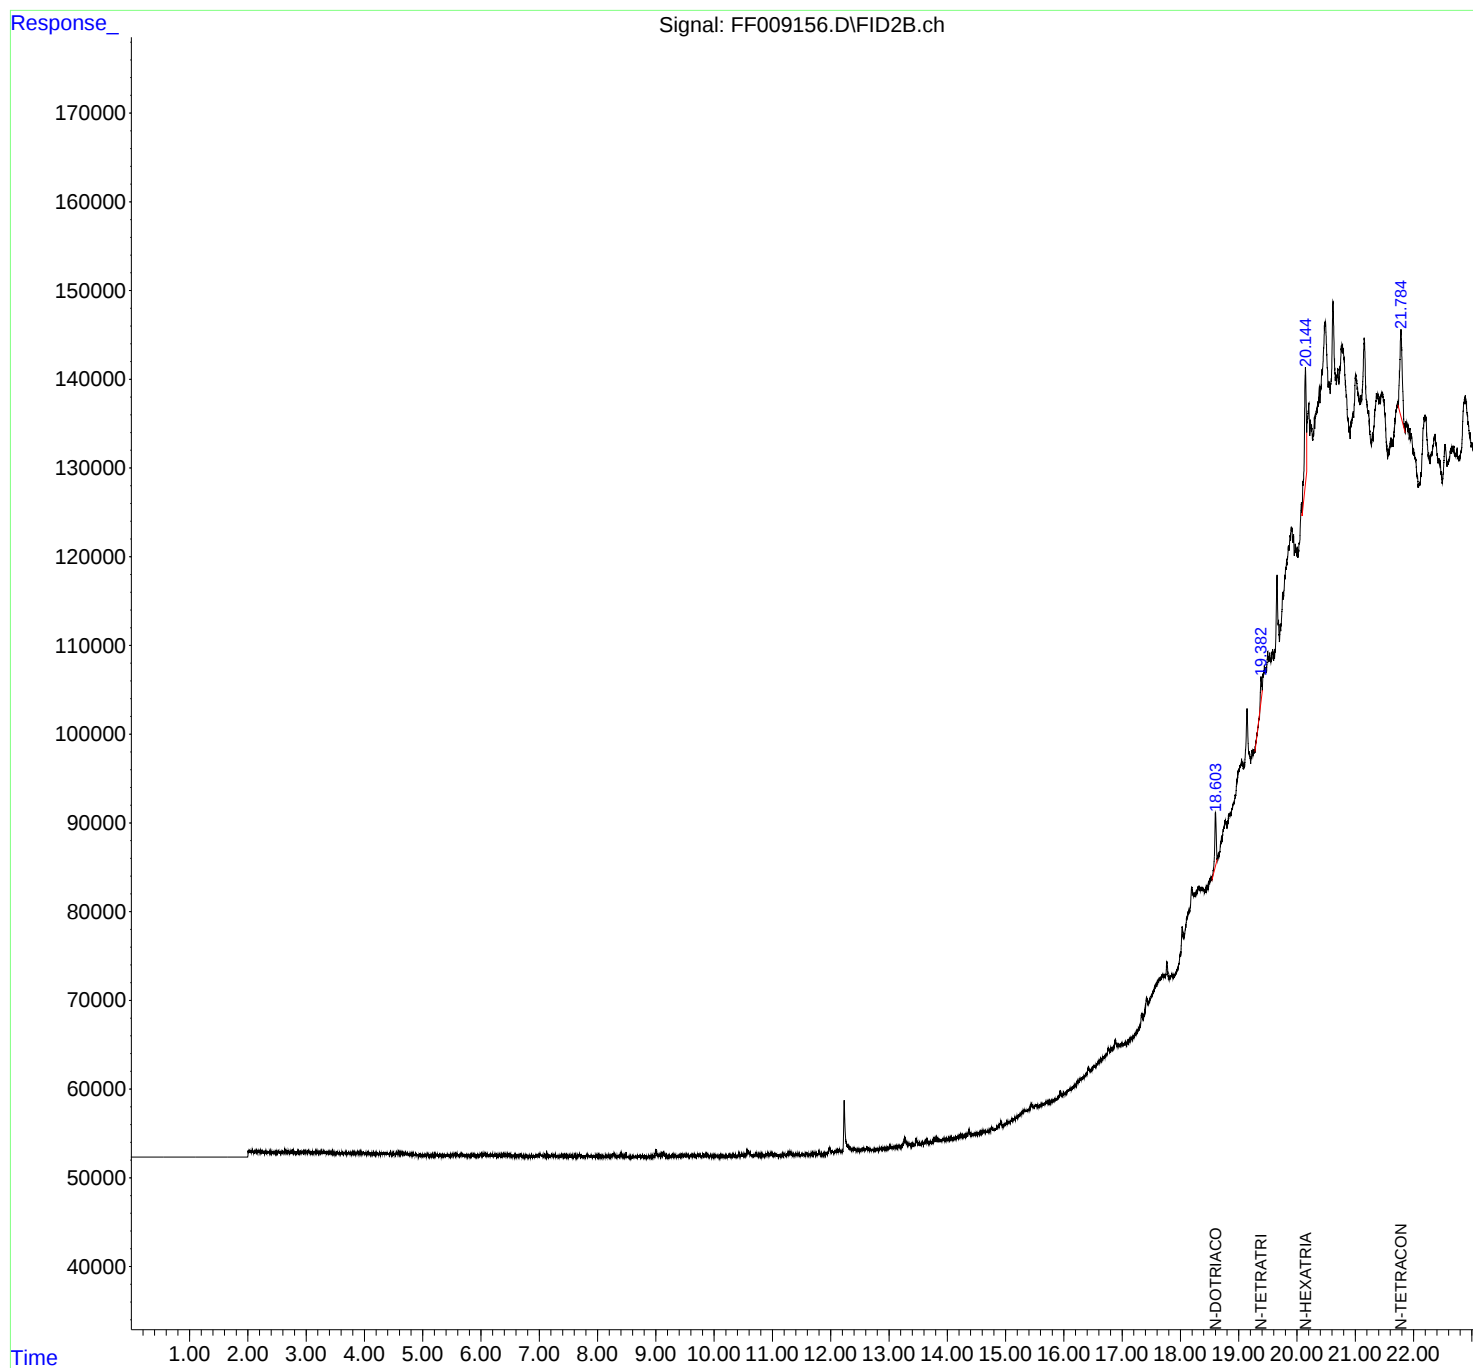


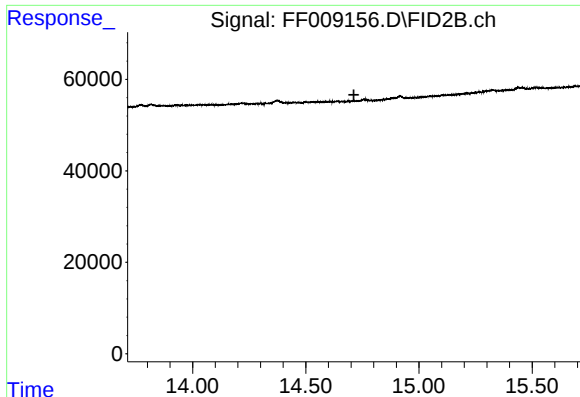

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.712 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

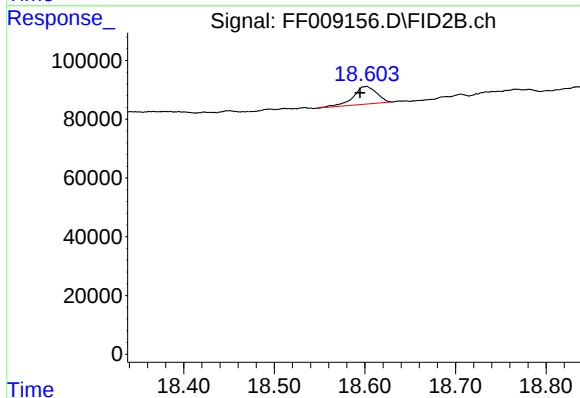


#14 N-DOTRIACONTANE

R.T.: 18.603 min
Delta R.T.: 0.008 min
Response: 107845
Conc: 1.02 ug/ml

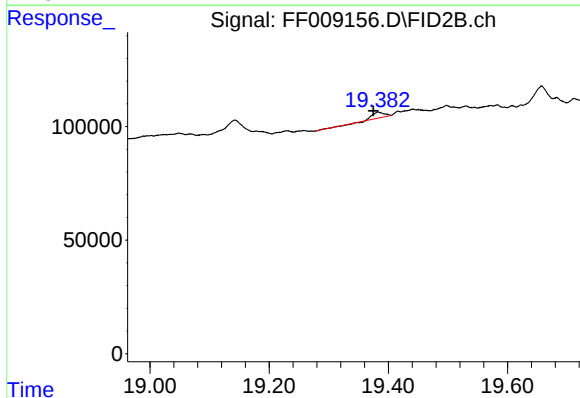


#15 N-TETRATRIACONTANE

R.T.: 19.383 min
Delta R.T.: 0.008 min
Response: 32445
Conc: 0.33 ug/ml

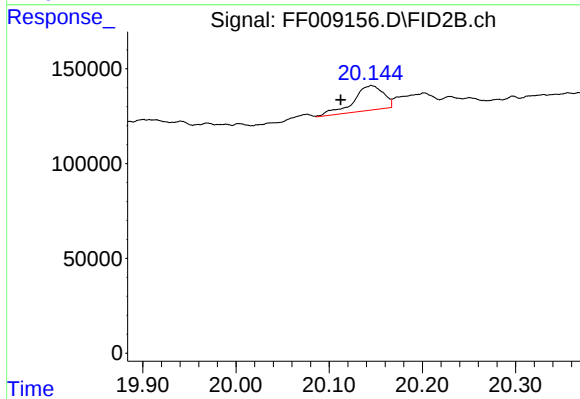

#16 N-HEXATRIACONTANE

R.T.: 20.145 min
Delta R.T.: 0.033 min
Response: 293865
Conc: 3.31 ug/ml

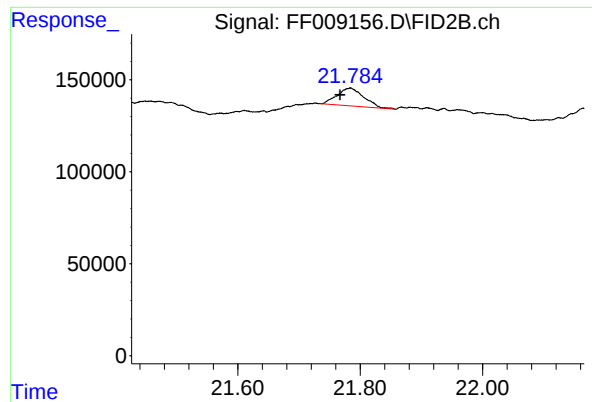

#18 N-TETRACONTANE

R.T.: 21.783 min
Delta R.T.: 0.016 min
Response: 292367
Conc: 3.60 ug/ml

Instrument :
FID_F
ClientSampleId :