

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101719\
Data File : FF005827.D
Signal(s) : FID2B.ch
Acq On : 17 Oct 2019 15:44
Operator : DD\AJ
Sample : K5406-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 18 00:37:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
Quant Title :
QLast Update : Thu Oct 03 04:07:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.672	2524740	19.418 ug/ml
Target Compounds			
4) N-TETRADECANE	8.286f	430086	2.737 ug/ml
12) N-OCTACOSANE	16.841	798417	5.606 ug/ml
13) N-TRIACONTANE	17.728	948135	6.827 ug/ml
14) N-DOTRIACONTANE	18.561	505531	3.773 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101719\
Data File : FF005827.D
Signal(s) : FID2B.ch
Acq On : 17 Oct 2019 15:44
Operator : DD\AJ
Sample : K5406-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 18 00:37:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
Quant Title :
QLast Update : Thu Oct 03 04:07:51 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

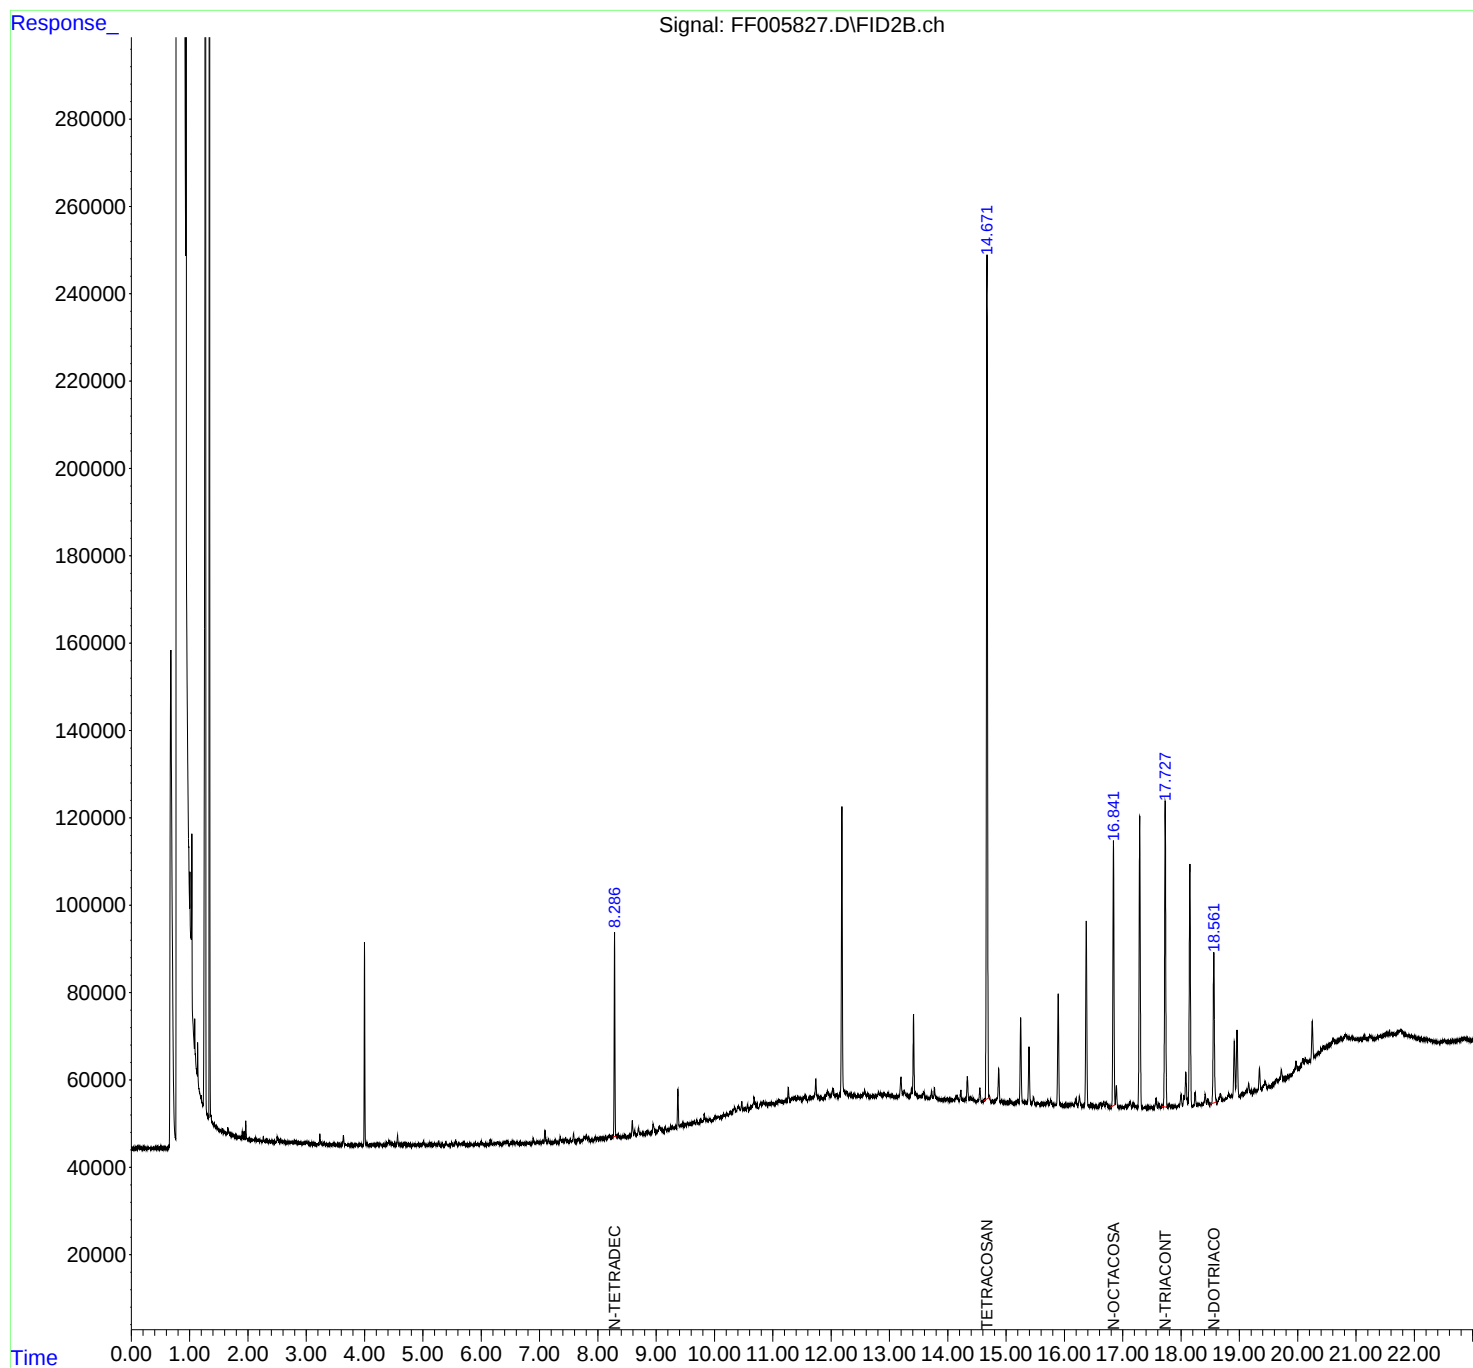

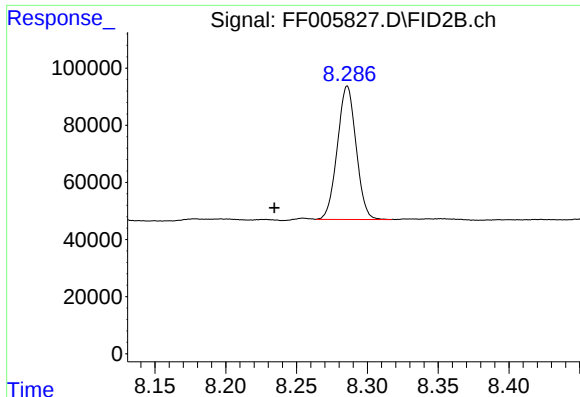


#4 N-TETRADECANE

R.T.: 8.286 min
Delta R.T.: 0.051 min
Response: 430086
Conc: 2.74 ug/ml

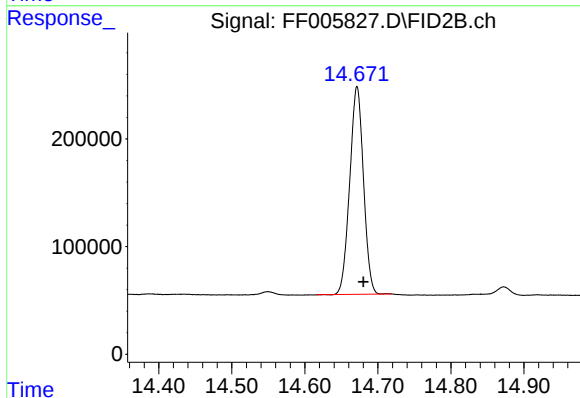


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.672 min
Delta R.T.: -0.009 min
Response: 2524740
Conc: 19.42 ug/ml

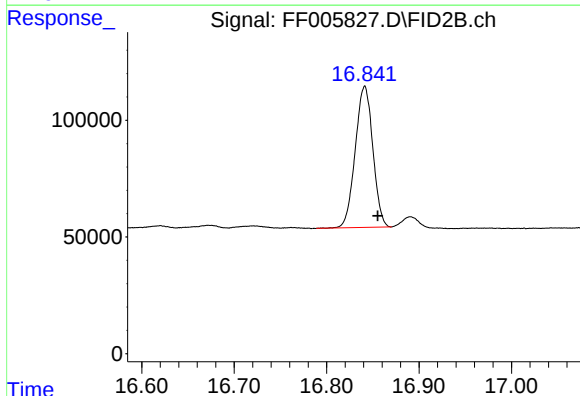


#12 N-OCTACOSANE

R.T.: 16.841 min
Delta R.T.: -0.014 min
Response: 798417
Conc: 5.61 ug/ml

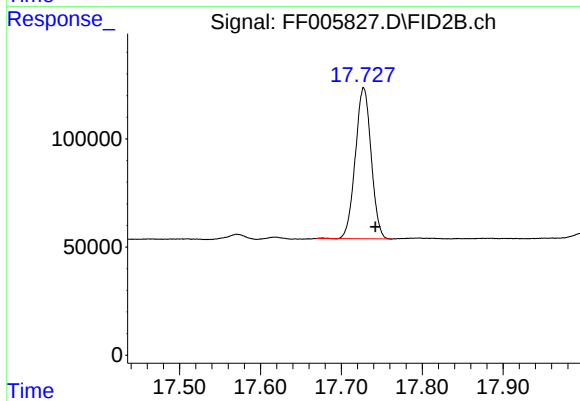

#13 N-TRIACONTANE

R.T.: 17.728 min
Delta R.T.: -0.014 min
Response: 948135
Conc: 6.83 ug/ml

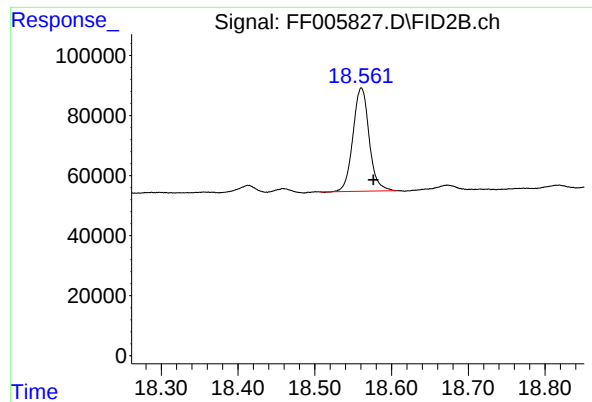

#14 N-DOTRIACONTANE

R.T.: 18.561 min
Delta R.T.: -0.016 min
Response: 505531
Conc: 3.77 ug/ml